



# ETHANOL GAS STANDARD CYLINDER REPORT

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
SFN 59282 (08/2018)

Chemical Test Operator Name (Print) GALLAGHER, JONATHAN		
Location HARV	Intoxilyzer® Serial Number 80-006500	
Gas Lot Number 34418080A2	Gas Cylinder Number 061	Gas Expiration Date 02/05/2021

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).  
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
  - A. 0.083 AC
  - B. 0.082 AC
  - C. 0.082 AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
  - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
  - B. ACA Test Record.

Chemical Test Operator Signature 	Date 26 FEB 19
Reviewed By (Crime Laboratory Use Only) 	Date 27 FEB 2019

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006500  
Location = HARU      8164.13.00 06/09  
02/26/2019      20:03

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	20:03
02 Std. Gas	0.083	20:04
03 Room Air	0.000	20:04
04 Std. Gas	0.082	20:04
05 Room Air	0.000	20:05
06 Std. Gas	0.082	20:05
07 Room Air	0.000	20:06


Lot No = 34418080A2

Cyl No = 61

Exp Date = 02/05/2021

County = 52

Oper No. = 131749

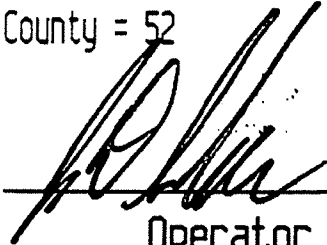

Operator Signature  
JONATHAN GALLAGHER

Remarks: