

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-003060 Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 230 psi Regulator: 250 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: DR3375 Lot #: 17160 Exp. Date: 6.8.19
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: DR7111 Lot #: 17150 Exp. Date: 10.11.19

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7089 Lot #: ICS 5 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 34917080A3 Cyl #: 28 Exp. Date: 2.5.20
Test 1 0.080 Test 4 0.080 Test 7 0.080
Test 2 0.081 Test 5 0.080 Test 8 0.080
Test 3 0.080 Test 6 0.080 Test 9 0.080
Average 0.080

C. Remarks/Maintenance: REPLACED SIMULATOR RETURN AND BREATH HOSE O-RINGS, ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ede
Breath Analyst Signature

4.10.2019
Date

NA
Reviewed by

NA
Date

Intoxilyzer Test Record and Checklist
 NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
 North Dakota Model 8000 SN 80-003060
 Location = TOXL 8164.14.00 09/16
 04/10/2019 13:25

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
 ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
 ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%&^*()_+?


Current Instrument Setup
 Data Entry Mode: Enabled
 Start Test Sequence: DABACABA
 Display Prelim Rslt? Yes
 Display Third Digit? Yes
 Inhib Printer(Y/N)? No
 Display Volume? No
 Disable On Memfull? Yes
 # of Print Copies? 1
 Select Std (D/W/I)? Dry
 Standard Value? 0.080
 Standard Lot #? 34917080A3
 Standard Cyl #? 28
 Standard Expiration? 02/05/2020
 Oper No? 666666

Flow Cal. Date: 04/08/2008
 Slope 702
 Intercept -647610

IR Calibration Date: 06/04/2008

	3um	9um
0th Coef(*100):	-5190	-7737
1st Coef(*100):	270580	138779
2nd Coef(*100):	2499	956
H2O adj(mg/l*10k):	377	188

***** Printer Test End *****



Operator Signature
 CHARLES EDER

Remarks: *PRINT TEST*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003060
Location = TOXL 8164.14.00 09/16
04/10/2019 13:48

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:49
02 Std. Sol.	0.020	13:50
03 Room Air	0.000	13:50
04 Std. Sol.	0.020	13:51
05 Room Air	0.000	13:52
06 Std. Sol.	0.021	13:52
07 Room Air	0.000	13:53


08 Sim Temp = 34.0°C

Simul Ser No = DR3375

Std Sol No = 17160

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003060
Location = TOXL 8164.14.00 09/16
04/10/2019 13:42

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:42
02 Std. Sol.	0.296	13:43
03 Room Air	0.000	13:43
04 Std. Sol.	0.297	13:44
05 Room Air	0.000	13:45
06 Std. Sol.	0.298	13:45
07 Room Air	0.000	13:46

08 Sim Temp = 34.0°C

Simul Ser No = DR7111
Std Sol No = ~~17160~~ CEE 17350
County = 08 Oper No. = 666666

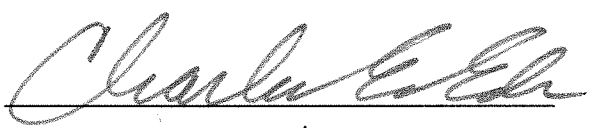

Operator Signature
CHARLES EDER

Remarks: HIGH AC
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003060
Location = TOXL 8164.14.00 09/16
04/10/2019 13:35

Test	AC	Time
01 Room Air	0.000	13:35
02 *Subject Test	INT*	13:36
03 Room Air	0.000	13:37

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 34917080A3
Cyl No = 28
Expiration Date = 02/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003060
Location = TOXL 8164.14.00 09/16
04/10/2019 13:31

Test	AC	Time
01 Diagnostic	OK	13:32
02 Room Air	RFI*	13:32
03 Room Air	0.000	13:33

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS821456
Lot No = 34917080A3
Cyl No = 28
Expiration Date = 02/05/2020
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003060
Location = TOXL 8164.14.00 09/16
04/10/2019 13:27

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:28
02 Std. Gas	0.080	13:28
03 Room Air	0.000	13:28
04 Std. Gas	0.081	13:29
05 Room Air	0.000	13:29
06 Std. Gas	0.080	13:30
07 Room Air	0.000	13:30

Lot No = 34917080A3
Cyl No = 28
Exp Date = 02/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *ACA TEST*
 0.080 AC

Form 106-I8000

CALIBRATION CHECK

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003060
Location = TOXL 8164.14.00 09/16
04/10/2019 13:54

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:55
02 Std. Gas	0.080	13:55
03 Room Air	0.000	13:56
04 Std. Gas	0.080	13:56
05 Room Air	0.000	13:57
06 Std. Gas	0.080	13:57
07 Room Air	0.000	13:58

Lot No = 34917080A3
Cyl No = 28
Exp Date = 02/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
ACA TEST 0.080

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003060
Location = TOXL 8164.14.00 09/16
04/10/2019 13:58

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:58
02 Std. Gas	0.080	13:59
03 Room Air	0.000	13:59
04 Std. Gas	0.080	14:00
05 Room Air	0.000	14:00
06 Std. Gas	0.080	14:00
07 Room Air	0.000	14:01

Lot No = 34917080A3
Cyl No = 28
Exp Date = 02/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

ACA CHECK
0.080 AC

Form 106-I8000

CALIBRATION CHECK