

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004950

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 492 psi Regulator: 500 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value \leq 0.03 AC: 0.015 AC
Sim. Ser #: DR5113 Lot #: 201805C Exp. Date: 5.30.20
- b. High AC (Level 1,C): Known Value \geq 0.25 AC: 0.300 AC
Sim. Ser #: DR7089 Lot #: 1735G Exp. Date: 10.11.19

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3451 Lot #: ICS 5 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 34418080A2 Cyl #: 45 Exp. Date: 2.5.21

Test 1	<u>0.081</u>	Test 4	<u>0.081</u>	Test 7	<u>0.081</u>
Test 2	<u>0.081</u>	Test 5	<u>0.081</u>	Test 8	<u>0.081</u>
Test 3	<u>0.080</u>	Test 6	<u>0.080</u>	Test 9	<u>0.081</u>
Average	<u>0.081</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Clinda E. Edr
Breath Analyst Signature

6.12.2019
Date

NA

NA

Reviewed by _____

Date _____

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/12/2019 15:05

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 45
Standard Expiration? 02/05/2021
Oper No? 666666

Flow Cal. Date: 01/18/2010
Slope 774
Intercept -908904

IR Calibration Date: 05/05/2016
 3um 9um

0th Coef(*100): -13717 -19495
1st Coef(*100): 271916 140513
2nd Coef(*100): 3504 1503
H2O adj(mg/l*10k): 370 426

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/12/2019 15:09

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:09
02 Std. Sol.	0.014	15:10
03 Room Air	0.000	15:10
04 Std. Sol.	0.014	15:11
05 Room Air	0.000	15:12
06 Std. Sol.	0.014	15:12
07 Room Air	0.000	15:13

08 Sim Temp = 34.0°C

Simul Ser No = DR5113
Std Sol No = 201805C
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC
0.015 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/12/2019 15:14

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:15
02 Std. Sol.	0.298	15:15
03 Room Air	0.000	15:16
04 Std. Sol.	0.300	15:17
05 Room Air	0.000	15:17
06 Std. Sol.	0.300	15:18
07 Room Air	0.000	15:18

08 Sim Temp = 34.0°C

Simul Ser No = DR7089
Std Sol No = 17350
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/12/2019 15:20

Test	AC	Time
01 Room Air	0.000	15:20
02 *Subject Test	INT*	15:21
03 Room Air	0.000	15:21

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 34418080A2
Cyl No = 45
Expiration Date = 02/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/12/2019 15:22

Test	AC	Time
01 Diagnostic	OK	15:22
02 Room Air	0.000	15:23
03 *Subject Test	RFI*	15:23
04 Room Air	0.000	15:23

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 34418080A2
Cyl No = 45
Expiration Date = 02/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/12/2019 15:24

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:24
02 Std. Gas	0.081	15:25
03 Room Air	0.000	15:25
04 Std. Gas	0.081	15:25
05 Room Air	0.000	15:26
06 Std. Gas	0.080	15:26
07 Room Air	0.000	15:27

Lot No = 34418080A2

Cyl No = 45

Exp Date = 02/05/2021

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/12/2019 15:27

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:28
02 Std. Gas	0.081	15:28
03 Room Air	0.000	15:28
04 Std. Gas	0.081	15:29
05 Room Air	0.000	15:29
06 Std. Gas	0.080	15:30
07 Room Air	0.000	15:30

Lot No = 34418080A2
Cyl No = 45
Exp Date = 02/05/2021
County = 08 Oper No. = 666666

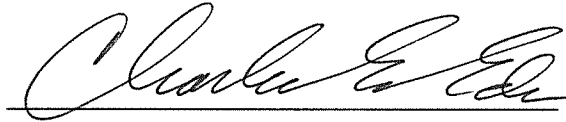

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/12/2019 15:30

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:31
02 Std. Gas	0.081	15:31
03 Room Air	0.000	15:32
04 Std. Gas	0.081	15:32
05 Room Air	0.000	15:33
06 Std. Gas	0.081	15:33
07 Room Air	0.000	15:33

Lot No = 34418080A2
Cyl No = 45
Exp Date = 02/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080AC

Form 106-I8000