



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
 SFN 59281 (06/2018)

Serial Number <b>80-005947</b>	Instrument Location <b>STARK LEC /DKPD</b>
Reason for Install/Repair <input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) <u>Repair request due to tone not working</u>	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): N/A (Tone worked properly)
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date <b>4/10/2020</b>
-------------------------------	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By 	Certified Date <b>4/16/20</b>
---------------------------	----------------------------------

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005947  
Location = DKPD                 8164.14.00 09/16  
04/10/2020                        01:32

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-=-|  
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-=-|  
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#\$\$%^&\*()\_+?

Current Instrument Setup

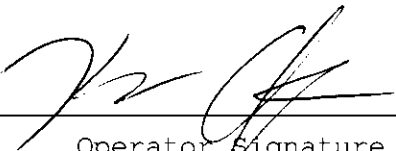
Data Entry Mode:                Enabled  
Start Test Sequence:            DABACABA  
Display Prelim Rslt?            Yes  
Display Third Digit?            Yes  
Inhib Printer(Y/N)?            No  
Display Volume?                No  
Disable On Memfull?            Yes  
# of Print Copies?              1  
Select Std (D/W/I)?            Dry  
Standard Value?                0.080  
Standard Lot #?                 34418080A2  
Standard Cyl #?                 11  
Standard Expiration?           02/05/2021  
Oper No?                        130935

Flow Cal. Date:                 06/21/2013  
Slope                            693  
Intercept                       -735360

IR Calibration Date:            04/06/2015

	3um	9um
0th Coef(*100):	-28096	-26982
1st Coef(*100):	280034	136042
2nd Coef(*100):	3530	1567
H2O adj(mg/l*10k):	510	437

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
-----  
Operator Signature  
KEVIN ELDRIDGE

Remarks:

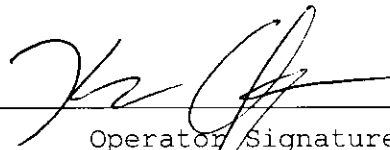
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005947  
Location = DKPD      8164.14.00 09/16  
04/10/2020      01:32

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	01:33
02 Std. Gas	0.080	01:33
03 Room Air	0.000	01:34
04 Std. Gas	0.080	01:34
05 Room Air	0.000	01:35
06 Std. Gas	0.079	01:35
07 Room Air	0.000	01:36

Lot No = 34418080A2  
Cyl No = 11  
Exp Date = 02/05/2021  
County = 45      Oper No. = 130935

  
Operator Signature  
KEVIN ELDRIDGE

Remarks:

Form 106-I8000

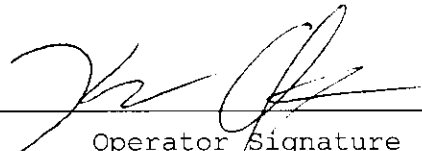
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005947  
Location = DKPD                8164.14.00 09/16  
04/10/2020                        01:36

Test	AC	Time
01 Room Air	0.000	01:38
02 *Subject Test	RFI*	01:38
03 Room Air	0.000	01:39

\*Invalid Test  
  Inhibited - RFI

Sub Name = TEST, TEST NA  
Sub DOB = 01/01/1999  
Sub Sex = Male                    Weight = 210  
Test = OTH                        Cit = 0000000000  
Dr. Lic. = ND/NA  
Lot No = 34418080A2  
Cyl No = 11  
Expiration Date = 02/05/2021  
County = 45                        Oper No. = 130935

  
\_\_\_\_\_  
Operator Signature  
KEVIN ELDRIDGE

Remarks:

Form 106-I8000