

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004956

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 325 psi Regulator: 400 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.015 AC
Sim. Ser #: MP3064 Lot #: 201805C Exp. Date: 5.30.20
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP3069 Lot #: 201902D Exp. Date: 2.20.21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3451 Lot #: ICSS Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 3441808A2 Cyl #: 5 Exp. Date: 2.5.21

Test 1	<u>0.081</u>	Test 4	<u>0.082</u>	Test 7	<u>0.082</u>
Test 2	<u>0.082</u>	Test 5	<u>0.082</u>	Test 8	<u>0.082</u>
Test 3	<u>0.082</u>	Test 6	<u>0.082</u>	Test 9	<u>0.081</u>
Average	<u>0.082</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Edr
Breath Analyst Signature

4.14.20
Date

NA

NA

Reviewed by _____

Date _____

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.14.00 09/16
04/14/2020 12:39

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=-|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=-|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 5
Standard Expiration? 02/05/2021
Oper No? 666666

Flow Cal. Date: 06/13/2019
Slope 606
Intercept -586035

IR Calibration Date: 06/13/2019
 3um 9um

0th Coef(*100): -19986 -21891
1st Coef(*100): 263289 136002
2nd Coef(*100): 2309 1332
H2O adj(mg/l*10k): 544 502

***** Printer Test End *****

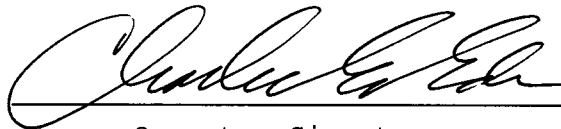

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.14.00 09/16
04/14/2020 12:46

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:47
02 Std. Sol.	0.015	12:48
03 Room Air	0.000	12:48
04 Std. Sol.	0.015	12:49
05 Room Air	0.000	12:49
06 Std. Sol.	0.016	12:50
07 Room Air	0.000	12:51

08 Sim Temp = 34.0°C

Simul Ser No = MP3064

Std Sol No = 201805C

County = 08

Oper No. = 666666



Operator Signature

CHARLES EDER

Remarks:

Low AC
0.015 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.14.00 09/16
04/14/2020 12:52

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:53
02 Std. Sol.	0.301	12:53
03 Room Air	0.000	12:54
04 Std. Sol.	0.303	12:55
05 Room Air	0.000	12:55
06 Std. Sol.	0.303	12:56
07 Room Air	0.000	12:57


08 Sim Temp = 34.0°C

Simul Ser No = MP3069

Std Sol No = 201902D

County = 08

Oper No. = 666666

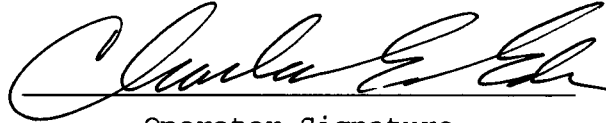

Operator Signature

CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.14.00 09/16
04/14/2020 12:41

Test	AC	Time
01 Room Air	0.000	12:41
02 *Subject Test	INT*	12:42
03 Room Air	0.000	12:43

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 34418080A2
Cyl No = 5
Expiration Date = 02/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.14.00 09/16
04/14/2020 12:43

Test	AC	Time
01 Diagnostic	OK	12:44
02 Room Air	0.000	12:44
03 *Subject Test	RFI*	12:44
04 Room Air	0.000	12:45

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 34418080A2
Cyl No = 5
Expiration Date = 02/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.14.00 09/16
04/14/2020 12:58

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:58
02 Std. Gas	0.081	12:59
03 Room Air	0.000	12:59
04 Std. Gas	0.082	13:00
05 Room Air	0.000	13:00
06 Std. Gas	0.082	13:01
07 Room Air	0.000	13:01

Lot No = 34418080A2
Cyl No = 5
Exp Date = 02/05/2021
County = 08 Oper No. = 666666

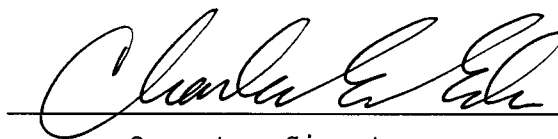

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.14.00 09/16
04/14/2020 13:01

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:02
02 Std. Gas	0.082	13:02
03 Room Air	0.000	13:03
04 Std. Gas	0.082	13:03
05 Room Air	0.000	13:04
06 Std. Gas	0.082	13:04
07 Room Air	0.000	13:05

Lot No = 34418080A2
Cyl No = 5
Exp Date = 02/05/2021
County = 08 Oper No. = 666666

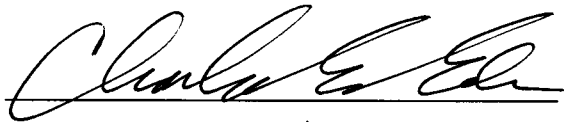

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.14.00 09/16
04/14/2020 13:05

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:06
02 Std. Gas	0.082	13:06
03 Room Air	0.000	13:07
04 Std. Gas	0.082	13:07
05 Room Air	0.000	13:07
06 Std. Gas	0.081	13:08
07 Room Air	0.000	13:08

Lot No = 34418080A2
Cyl No = 5
Exp Date = 02/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000