

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004193

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 345 psi Regulator: 350 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.015 AC
Sim. Ser #: MP3064 Lot #: 201805C Exp. Date: 5.30.20
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP3069 Lot #: 201902D Exp. Date: 2.20.21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3451 Lot #: ICSS Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 05620080A1 Cyl #: 47 Exp. Date: 4.5.22
Test 1 0.078 Test 4 0.079 Test 7 0.079
Test 2 0.079 Test 5 0.079 Test 8 0.079
Test 3 0.078 Test 6 0.079 Test 9 0.079
Average 0.079

C. Remarks/Maintenance: ANNUAL INSPECTION

CLASSROOM ONLY UNTIL EVALUATED/REPAIRED. AUTORANGE VALUE LOW.

Instrument is acceptable to be used in the field.

Breath Analyst Signature

Charles E. Eck

NA

Date

5/4/20

NA

Reviewed by

Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
05/04/2020 11:29

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 05620080A1
Standard Cyl #? 47
Standard Expiration? 04/05/2022
Oper No? 666666

Flow Cal. Date: 06/18/2019
Slope 622
Intercept -723749

IR Calibration Date: 06/18/2019
 3um 9um

0th Coef(*100): -14782 -15525
1st Coef(*100): 267622 134211
2nd Coef(*100): 2469 1112
H2O adj(mg/l*10k): 264 225

***** Printer Test End *****

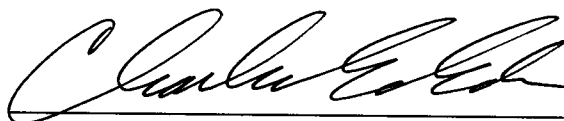

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
05/04/2020 11:33

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:33
02 Std. Sol.	0.013	11:34
03 Room Air	0.000	11:35
04 Std. Sol.	0.014	11:35
05 Room Air	0.000	11:36
06 Std. Sol.	0.014	11:37
07 Room Air	0.000	11:37

08 Sim Temp = 34.0°C

Simul Ser No = MP3064

Std Sol No = 201805C

County = 08

Oper No. = 666666



Operator Signature

CHARLES EDER

Remarks:

LOW AC
0.015 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
05/04/2020 13:26

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:26
02 Std. Sol.	0.304	13:27
03 Room Air	0.000	13:28
04 Std. Sol.	0.305	13:28
05 Room Air	0.000	13:29
06 Std. Sol.	0.302	13:30
07 Room Air	0.000	13:30

08 Sim Temp = 34.0°C

Simul Ser No = MP3069

Std Sol No = 201902D

County = 08

Oper No. = 666666



Operator Signature

CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
05/04/2020 13:33

Test	AC	Time
01 Room Air	0.000	13:34
02 *Subject Test	INT*	13:34
03 Room Air	0.000	13:35

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 05620080A1
Cyl No = 47
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
05/04/2020 13:35

Test	AC	Time
01 Diagnostic	OK	13:36
02 Room Air	0.000	13:36
03 *Subject Test	RFI*	13:37
04 Room Air	0.000	13:37

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 05620080A1
Cyl No = 47
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
05/04/2020 13:49

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:49
02 Std. Gas	0.078	13:49
03 Room Air	0.000	13:50
04 Std. Gas	0.079	13:50
05 Room Air	0.000	13:51
06 Std. Gas	0.078	13:51
07 Room Air	0.000	13:52

Lot No = 05620080A1
Cyl No = 47
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

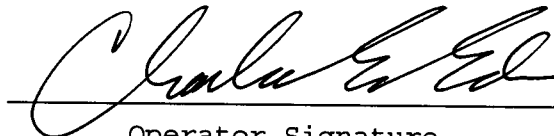

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
05/04/2020 13:52

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:52
02 Std. Gas	0.079	13:53
03 Room Air	0.000	13:53
04 Std. Gas	0.079	13:54
05 Room Air	0.000	13:54
06 Std. Gas	0.079	13:55
07 Room Air	0.000	13:55

Lot No = 05620080A1
Cyl No = 47
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

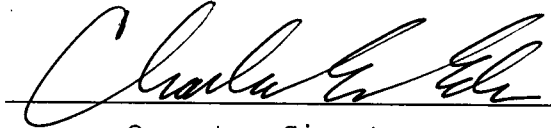

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
05/04/2020 13:55

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:56
02 Std. Gas	0.079	13:56
03 Room Air	0.000	13:57
04 Std. Gas	0.079	13:57
05 Room Air	0.000	13:58
06 Std. Gas	0.079	13:58
07 Room Air	0.000	13:59

Lot No = 05620080A1
Cyl No = 47
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

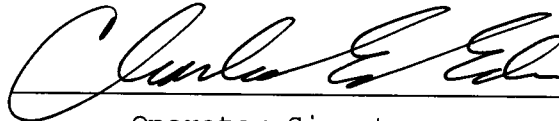

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK

0.080 AC

Form 106-I8000