

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004188

Location: TOXL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 923 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.020 AC  
Sim. Ser #: MP5321 Lot #: 2018100 Exp. Date: 10-24-20
- b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.250 AC  
Sim. Ser #: MP5290 Lot #: 201911B Exp. Date: 11-5-21

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR734B Lot #: 1055 Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 24119080A1 Cyl #: 006 Exp. Date: 11-09-21

Test 1 <u>0.079</u>	Test 4 <u>0.080</u>	Test 7 <u>0.079</u>
Test 2 <u>0.080</u>	Test 5 <u>0.080</u>	Test 8 <u>0.080</u>
Test 3 <u>0.080</u>	Test 6 <u>0.079</u>	Test 9 <u>0.079</u>
Average <u>0.079</u>		

C. Remarks/Maintenance: Annual inspection

TRAINING FOR KALI HEB. CEE 5/6/20

Instrument is acceptable to be used in the field

Kali L. Hieb / Charles E. Ee  
Breath Analyst Signature

5.6.2020  
06 May 20  
Date

Charles E. Ee  
Reviewed by

5.6.2020  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004188  
Location = TOXL                    8164.14.00 09/16  
05/06/2020                            14:10

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup

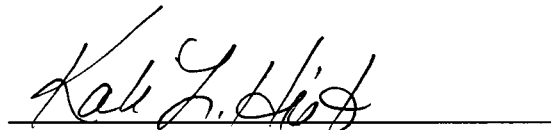
Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            05620080A1  
Standard Cyl #?            048  
Standard Expiration?       04/05/2022  
Oper No?                    123456

Flow Cal. Date:            04/30/2020  
Slope                        645  
Intercept                   -637424

IR Calibration Date:        05/06/2020

	3um	9um
0th Coef(*100):	-30092	-33449
1st Coef(*100):	293453	143538
2nd Coef(*100):	151	602
H2O adj(mg/l*10k):	425	462

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
N/A STUDENT

Remarks:

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004188  
Location = TOXL      8164.14.00 09/16  
05/06/2020      14:17

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:17
02 Std. Sol.	0.021	14:19
03 Room Air	0.000	14:19
04 Std. Sol.	0.020	14:20
05 Room Air	0.000	14:20
06 Std. Sol.	0.020	14:21
07 Room Air	0.000	14:22

08 Sim Temp = 33.9°C

Simul Ser No = MP5321  
Std Sol No = 201810D  
County = 08      Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks: *Calibration check*  
*Low AC 0.020 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

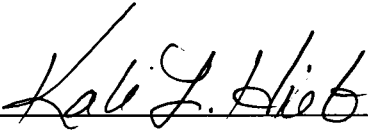
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004188  
Location = TOXL                    8164.14.00 09/16  
05/06/2020                            14:24

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:25
02 Std. Sol.	0.258	14:26
03 Room Air	0.000	14:26
04 Std. Sol.	0.258	14:27
05 Room Air	0.000	14:28
06 Std. Sol.	0.257	14:28
07 Room Air	0.000	14:29

08 Sim Temp = 34.0°C

Simul Ser No = MP5290  
Std Sol No = 201911B  
County = 08                            Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks: *Calibration check*  
*High AC 0.250 AC*  
Form 106-I8000

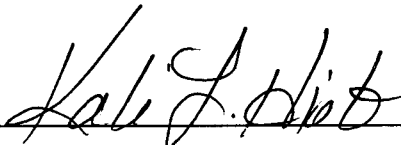
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004188  
Location = TOXL                8164.14.00 09/16  
05/06/2020                        14:38

Test	AC	Time
01 Room Air	0.000	14:39
02 *Subject Test	INT*	14:40
03 Room Air	0.000	14:41

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 13518100A3  
Cyl No = 006  
Expiration Date = 08/05/2020  
County = 08                          Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks: *Interferent Check*  
*0.10 AC + 0.059% Acetone*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

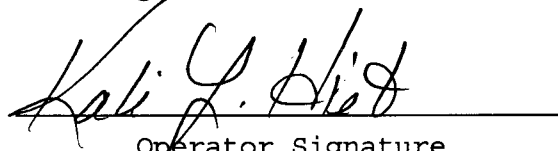
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004188  
Location = TOXL                    8164.14.00 09/16  
05/06/2020                            14:42

Test	AC	Time
01 Diagnostic	OK	14:44
02 Room Air	RFI*	14:44
03 Room Air	0.000	14:45

\*Invalid Test  
  Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 13518100A3  
Cyl No = 006  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 123456

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
N/A STUDENT

Remarks: *RFI check*

Form 106-I8000

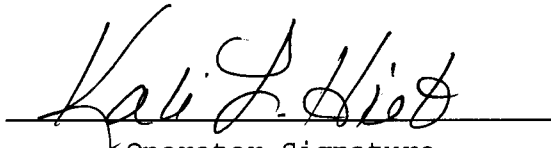
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004188  
Location = TOXL                    8164.14.00 09/16  
05/06/2020                            15:09

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:09
02 Std. Gas	0.079	15:10
03 Room Air	0.000	15:10
04 Std. Gas	0.080	15:11
05 Room Air	0.000	15:11
06 Std. Gas	0.080	15:12
07 Room Air	0.000	15:12

Lot No = 24119080A1  
Cyl No = 006  
Exp Date = 11/05/2021  
County = 08                            Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks: *Calibration check*  
*0.080 AC*  
Form 106-I8000

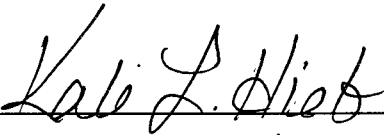
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004188  
Location = TOXL                    8164.14.00 09/16  
05/06/2020                            15:15

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:15
02 Std. Gas	0.080	15:16
03 Room Air	0.000	15:16
04 Std. Gas	0.080	15:17
05 Room Air	0.000	15:17
06 Std. Gas	0.079	15:17
07 Room Air	0.000	15:18

Lot No = 24119080A1  
Cyl No = 006  
Exp Date = 11/05/2021  
County = 08                            Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks: *Calibration check*  
*0.080 AC*

Form 106-I8000



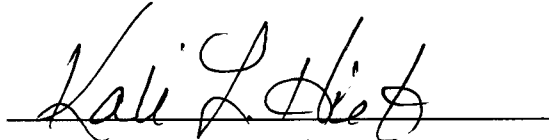
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004188  
Location = TOXL      8164.14.00 09/16  
05/06/2020      15:19

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:20
02 Std. Gas	0.079	15:20
03 Room Air	0.000	15:20
04 Std. Gas	0.080	15:21
05 Room Air	0.000	15:21
06 Std. Gas	0.079	15:22
07 Room Air	0.000	15:22

Lot No = 24119080A1  
Cyl No = 006  
Exp Date = 11/05/2021  
County = 08      Oper No. = 123456

  
Operator Signature  
N/A STUDENT

Remarks: *Calibration check*  
*D.DBo AC*  
Form 106-I8000