

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004197

Location: TOYL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi. <sup>KLH</sup> 4-18-20  
a. Display: 742 psi Regulator: 740 psi Low AC Known Value

B. Tests (Sign and attach test records):

- Configure simulator for the following tests (Level 1,S). <sup>KLH</sup> 4-18-20  
Sim Ser # MP532 P-020AC  
Lot # 201810A  
Exp. 10.24.20
1. Wet Calibration Check  
a.  Low AC (Level 1,C): Known Value  $\leq$  0.03 AC: 0.010 AC  
Sim. Ser #: MP5320 Lot #: 201805B Exp. Date: 5.30.20  
b.  High AC (Level 1,C): Known Value  $\geq$  0.25 AC: 0.250 AC  
Sim. Ser #: MP5290 Lot #: 201911B Exp. Date: 11.5.21

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR734B Lot #: LC55 Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 056200B0A1 Cyl #: 048 Exp. Date: 4.5.2022  
Test 1 0.078 Test 4 0.080 Test 7 0.079  
Test 2 0.078 Test 5 0.078 Test 8 0.078  
Test 3 0.078 Test 6 0.078 Test 9 0.078  
Average 0.078

C. Remarks/Maintenance: Annual Inspection  
Classroom only, flow sensor issue.  
TRAINING FOR KALI HIEB. CEE

Instrument is acceptable to be used in the field.

Breath Analyst Signature

Reviewed by

Date

Date

02/18

Issuing Authority - CEE

Page 1 of 1

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer          Alcohol Analyzer  
North Dakota Model 8000         SN 80-004197  
Location = TOXL                    8164.14.00 09/16  
06/03/2020                                  15:29

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstu vwxyz1234567890- = |  
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^ &\* ( ) \_ + ?

abcdefghijklmnopqrstu vwxyz1234567890- = |  
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^ &\* ( ) \_ + ?

Current Instrument Setup


Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?             34418080A2  
Standard Cyl #?             40  
Standard Expiration?       02/05/2021  
Oper No?                    123456

Flow Cal. Date:            06/26/2019  
Slope                        567  
Intercept                    293062

IR Calibration Date:       09/19/2016  
    3um                                  9um

-----  
0th Coef(\*100):          -15020                                  -25720  
1st Coef(\*100):          274116                                 137966  
2nd Coef(\*100):          1298                                     699  
H2O adj(mg/l\*10k):       226                                     399

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
N/A STUDENT

Remarks: *print test*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

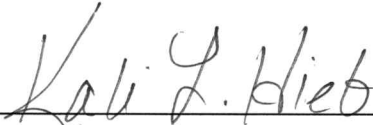
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004197  
Location = TOXL      8164.14.00 09/16  
06/03/2020      15:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:34
02 Std. Sol.	0.009	15:36
03 Room Air	0.000	15:36
04 Std. Sol.	0.010	15:37
05 Room Air	0.000	15:37
06 Std. Sol.	0.010	15:38
07 Room Air	0.000	15:38

08 Sim Temp = 34.0°C

Simul Ser No = MP5320  
Std Sol No = 201805B  
County = 08      Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks:      cal check 0.010AC  
                                low AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

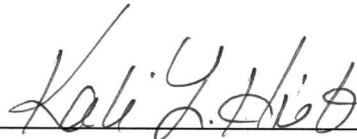
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004197  
Location = TOXL                    8164.14.00 09/16  
06/03/2020                            15:41

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:41
02 Std. Sol.	0.249	15:42
03 Room Air	0.000	15:43
04 Std. Sol.	0.250	15:44
05 Room Air	0.000	15:44
06 Std. Sol.	0.249	15:45
07 Room Air	0.000	15:46

08 Sim Temp = 34.0°C

Simul Ser No = MP5290  
Std Sol No = 201911B  
County = 08                            Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks: *High AC 0.250 AC*  
*Cal check*

Form 106-I8000

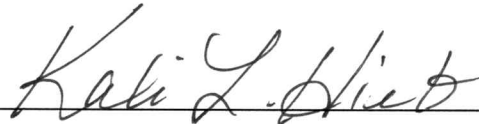
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004197  
Location = TOXL                    8164.14.00 09/16  
06/03/2020                            15:49

Test	AC	Time
01 Room Air	0.000	15:50
02 *Subject Test	INT*	15:51
03 Room Air	0.000	15:51

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 05620080A1  
Cyl No = 048  
Expiration Date = 04/05/2022  
County = 08                          Oper No. = 123456

  
Operator Signature  
N/A STUDENT

Remarks: *Interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

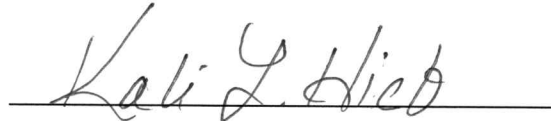
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004197  
Location = TOXL                    8164.14.00 09/16  
06/03/2020                            15:52

Test	AC	Time
01 Diagnostic	OK	15:53
02 Room Air	RFI*	15:54
03 Room Air	0.000	15:54

\*Invalid Test  
  Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 05620080A1  
Cyl No = 048  
Expiration Date = 04/05/2022  
County = 08                          Oper No. = 123456

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
N/A STUDENT

Remarks:

*RFI Check*

Form 106-I8000

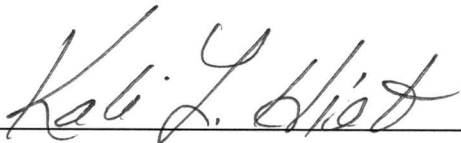
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004197  
Location = TOXL      8164.14.00 09/16  
06/03/2020      15:55

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:56
02 Std. Gas	0.078	15:56
03 Room Air	0.000	15:56
04 Std. Gas	0.078	15:57
05 Room Air	0.000	15:57
06 Std. Gas	0.078	15:58
07 Room Air	0.000	15:58

Lot No = 05620080A1  
Cyl No = 048  
Exp Date = 04/05/2022  
County = 08      Oper No. = 123456

  
Operator Signature  
N/A STUDENT

Remarks: *cal check 0.000 AC*

Form 106-I8000

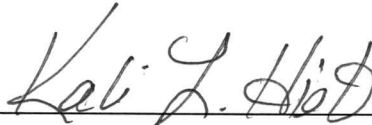
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004197  
Location = TOXL      8164.14.00 09/16  
06/03/2020      15:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:59
02 Std. Gas	0.080	15:59
03 Room Air	0.000	16:00
04 Std. Gas	0.078	16:00
05 Room Air	0.000	16:01
06 Std. Gas	0.078	16:01
07 Room Air	0.000	16:02

Lot No = 05620080A1  
Cyl No = 048  
Exp Date = 04/05/2022  
County = 08      Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks: *Cal check 0.080 AC*

Form 106-I8000



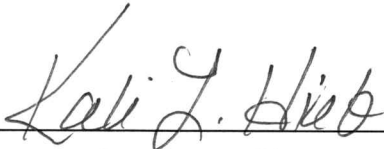
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004197  
Location = TOXL      8164.14.00 09/16  
06/03/2020      16:03

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:03
02 Std. Gas	0.079	16:04
03 Room Air	0.000	16:04
04 Std. Gas	0.078	16:05
05 Room Air	0.000	16:05
06 Std. Gas	0.078	16:05
07 Room Air	0.000	16:06

Lot No = 05620080A1  
Cyl No = 048  
Exp Date = 04/05/2022  
County = 08      Oper No. = 123456

  
\_\_\_\_\_  
Operator Signature  
N/A STUDENT

Remarks: *Cal check 0.080 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

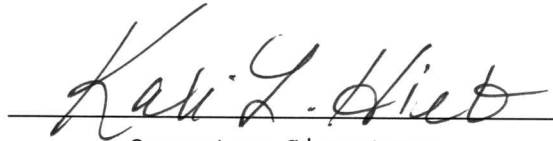
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004197  
Location = TOXL                    8164.14.00 09/16  
06/18/2020                            10:07

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:08
02 Std. Sol.	0.019	10:09
03 Room Air	0.000	10:09
04 Std. Sol.	0.019	10:10
05 Room Air	0.000	10:10
06 Std. Sol.	0.020	10:11
07 Room Air	0.000	10:11

08 Sim Temp = 33.9°C

Simul Ser No = MP5321  
Std Sol No = 201810D  
County = 08                            Oper No. = 123456

  
Operator Signature  
N/A STUDENT

Remarks: *cal check*  
*low ac 0.020 ac*

Form 106-I8000