

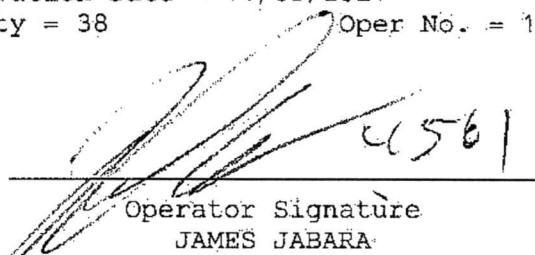
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = MOHL 8164.14.00 09/16
06/29/2020 21:22

Test	AC	Time
01 Room Air	0.000	21:26
02 *Subject Test	RFI*	21:26
03 Room Air	RFI*	21:26

*Invalid Test
Inhibited - RFI

Sub Name = JOHN, DOE NA
Sub DOB = 11/22/1988
Sub Sex = Male Weight = 220
Test = OTH Cit. = 000000000000
Dr. Lic. = ND/000000
Lot No = 24119080A1
Cyl No = 34
Expiration Date = 11/05/2021
County = 38 Oper No. = 131544

 4561
Operator Signature
JAMES JABARA

Remarks:

Form 106-18000