

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-005941

Location: TOXL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 897 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.015 AC  
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.400 AC  
Sim. Ser #: MP3062 Lot #: 202103E Exp. Date: 3-24-23

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR3451 Lot #: ICS 6 Exp. Date: NA

Display reads "Interferent Detect"

3.  RFI Check (CMS Mode)  Display reads "RFI Detect"

4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC CEE  
Gas Cyl Lot #: 24119080A1 Cyl #: 5 Exp. Date: 11-05-21  
Test 1 0.083 Test 4 0.083 Test 7 0.083  
Test 2 0.082 Test 5 0.083 Test 8 0.082  
Test 3 0.083 Test 6 0.082 Test 9 0.082  
Average 0.083

C. Remarks/Maintenance: ANNUAL INSPECTION

CLASSROOM ONLY INSTRUMENT - AUTO CAL ISSUE WITH CALIBRATION ADJUSTMENT

Instrument is acceptable to be used in the field. NO

Breath Analyst Signature

Reviewed by

Date

Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005941  
Location = TOXL                 8164.14.00 09/16  
04/12/2021                        15:49

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup


Data Entry Mode:                Enabled  
Start Test Sequence:            DABACABA  
Display Prelim Rslt?            Yes  
Display Third Digit?            Yes  
Inhib Printer(Y/N)?            No  
Display Volume?                No  
Disable On Memfull?            Yes  
# of Print Copies?              1  
Select Std (D/W/I)?            Dry  
Standard Value?                0.080  
Standard Lot #?                 24119080A1  
Standard Cyl #?                5  
Standard Expiration?            11/05/2021  
Oper No?                        666666

Flow Cal. Date:                 05/30/2018  
Slope                            618  
Intercept                        -570330

IR Calibration Date:            05/30/2018

	3um	9um
0th Coef(*100):	-13785	-15807
1st Coef(*100):	281869	139821
2nd Coef(*100):	2733	1395
H2O adj(mg/l*10k):	308	362

\*\*\*\*\* Printer Test End \*\*\*\*\*

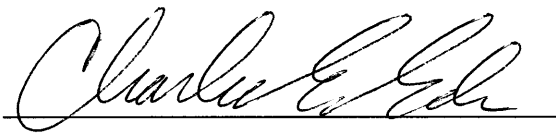

Operator Signature  
CHARLES EDER

Remarks: **PRINT TEST**

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005941  
Location = TOXL                    8164.14.00 09/16  
04/12/2021                            15:50

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:51
02 Std. Sol.	0.014	15:52
03 Room Air	0.000	15:52
04 Std. Sol.	0.015	15:53
05 Room Air	0.000	15:53
06 Std. Sol.	0.016	15:54
07 Room Air	0.000	15:55

08 Sim Temp = 34.0°C

Simul Ser No = MP5319  
Std Sol No = 201911C  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:    *Low AC*  
                  *0.015 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005941  
Location = TOXL      8164.14.00 09/16  
04/12/2021      15:56

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:56
02 Std. Sol.	0.412	15:57
03 Room Air	0.000	15:58
04 Std. Sol.	0.413	15:58
05 Room Air	0.000	15:59
06 Std. Sol.	0.412	16:00
07 Room Air	0.000	16:00


08 Sim Temp = 34.0°C

Simul Ser No = MP3062

Std Sol No = 202103E

County = 08

Oper No. = 666666

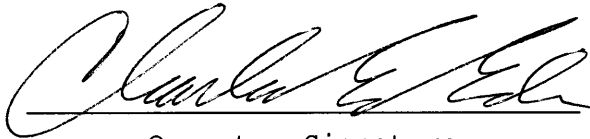

Operator Signature

CHARLES EDER

Remarks:

HIGH AC  
0.400 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005941  
Location = TOXL                 8164.14.00 09/16  
04/12/2021                        16:02

Test	AC	Time
01 Room Air	0.000	16:03
02 *Subject Test	INT*	16:03
03 Room Air	0.000	16:04

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 02/01/1992  
Sub Sex = Female                 Weight = 150  
Test = DUI                        Cit = INTERFERENT  
Dr. Lic. = ND/DIS921456  
Lot No = 24119080A1  
Cyl No = 5  
Expiration Date = 11/05/2021  
County = 08                        Oper No. = 666666



Operator Signature  
CHARLES, EDER

Remarks:

*Interferent Check*  
~~0.100~~ 0.10 AC + 0.05% ACETONE  
CEE

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005941  
Location = TOXL      8164.14.00 09/16  
04/12/2021      16:07

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:07
02 Std. Gas	0.083	16:08
03 Room Air	0.000	16:08
04 Std. Gas	0.082	16:09
05 Room Air	0.000	16:09
06 Std. Gas	0.083	16:09
07 Room Air	0.000	16:10

Lot No = 24119080A1  
Cyl No = 5  
Exp Date = 11/05/2021  
County = 08      Oper No. = 666666

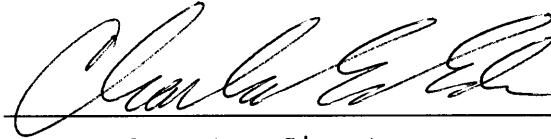

Operator Signature  
CHARLES EDER

Remarks:

CALIBRATION CHECK  
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005941  
Location = TOXL      8164.14.00 09/16  
04/12/2021      16:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:11
02 Std. Gas	0.083	16:11
03 Room Air	0.000	16:12
04 Std. Gas	0.083	16:12
05 Room Air	0.000	16:12
06 Std. Gas	0.082	16:13
07 Room Air	0.000	16:13

Lot No = 24119080A1  
Cyl No = 5  
Exp Date = 11/05/2021  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005941  
Location = TOXL      8164.14.00 09/16  
04/12/2021      16:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:14
02 Std. Gas	0.083	16:14
03 Room Air	0.000	16:15
04 Std. Gas	0.082	16:15
05 Room Air	0.000	16:16
06 Std. Gas	0.082	16:16
07 Room Air	0.000	16:17

Lot No = 24119080A1  
Cyl No = 5  
Exp Date = 11/05/2021  
County = 08      Oper No. = 666666

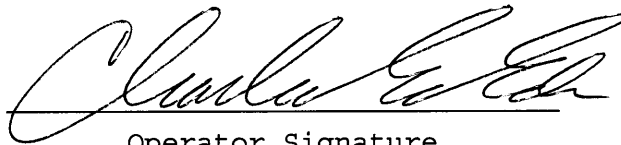

Operator Signature  
CHARLES EDER

Remarks:

CALIBRATION CHECK  
0.080 AC

Form 106-I8000