

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004193

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 426 psi Regulator: 400 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3451 Lot #: ICS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 24119080A1 Cyl #: 6 Exp. Date: 11.5.21

Test 1	<u>0.080</u>	Test 4	<u>0.080</u>	Test 7	<u>0.080</u>
Test 2	<u>0.080</u>	Test 5	<u>0.080</u>	Test 8	<u>0.080</u>
Test 3	<u>0.080</u>	Test 6	<u>0.080</u>	Test 9	<u>0.080</u>
Average	<u>0.080</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

CLASSROOM ONLY INSTRUMENT - AUTO RANGE ISSUE DURING CALIBRATION ADJUST

Instrument is acceptable to be used in the field. NO

Breath Analyst Signature

Reviewed by

Date

Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
04/12/2021 12:30

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 6
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 06/18/2019
Slope 622
Intercept -723749

IR Calibration Date: 06/18/2019
 3um 9um

0th Coef(*100): -14782 -15525
1st Coef(*100): 267622 134211
2nd Coef(*100): 2469 1112
H2O adj(mg/l*10k): 264 225

***** Printer Test End *****

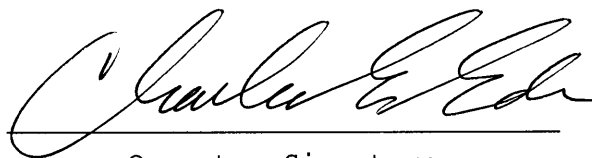

Operator Signature
CHARLES EDER

Remarks: PRINT TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
04/12/2021 12:33

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:33
02 Std. Sol.	0.020	12:34
03 Room Air	0.000	12:35
04 Std. Sol.	0.021	12:35
05 Room Air	0.000	12:36
06 Std. Sol.	0.021	12:37
07 Room Air	0.000	12:37


08 Sim Temp = 34.0°C

Simul Ser No = MP3064

Std Sol No = 20070

County = 08

Oper No. = 666666

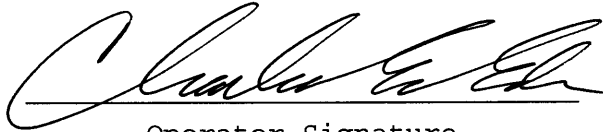

Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
04/12/2021 12:44

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:44
02 Std. Sol.	0.311	12:45
03 Room Air	0.000	12:46
04 Std. Sol.	0.311	12:46
05 Room Air	0.000	12:47
06 Std. Sol.	0.310	12:48
07 Room Air	0.000	12:48


08 Sim Temp = 34.0°C

Simul Ser No = MP5317

Std Sol No = 202012A

County = 08

Oper No. = 666666

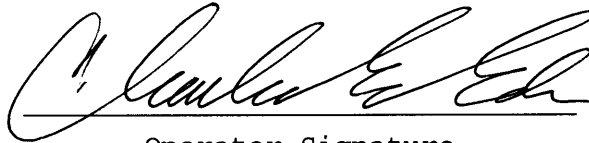

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
04/12/2021 12:51

Test	AC	Time
01 Room Air	0.000	12:52
02 *Subject Test	INT*	12:52
03 Room Air	0.000	12:53

*Invalid Test
Interferent Detected

Sub Name = BILLS, THE BUFFALO
Sub DOB = 06/14/1993
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/BIL933277
Lot No = 24119080A1
Cyl No = 6
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

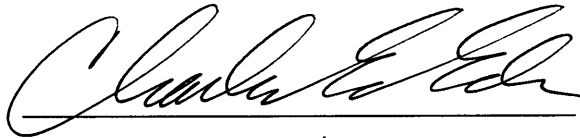

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10 AC + 0.05% ACETONE
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
04/12/2021 12:53

Test	AC	Time
01 Diagnostic	OK	12:54
02 Room Air	0.000	12:54
03 *Subject Test	RFI*	12:54
04 Room Air	0.000	12:55

*Invalid Test
Inhibited - RFI

Sub Name = BILLS, THE BUFFALO
Sub DOB = 06/14/1993
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/BIL933277
Lot No = 24119080A1
Cyl No = 6
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
04/12/2021 12:55

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:56
02 Std. Gas	0.080	12:56
03 Room Air	0.000	12:57
04 Std. Gas	0.080	12:57
05 Room Air	0.000	12:58
06 Std. Gas	0.080	12:58
07 Room Air	0.000	12:59

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

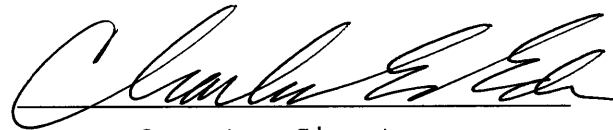

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
04/12/2021 12:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:59
02 Std. Gas	0.080	13:00
03 Room Air	0.000	13:00
04 Std. Gas	0.080	13:01
05 Room Air	0.000	13:01
06 Std. Gas	0.080	13:02
07 Room Air	0.000	13:02

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *CALIBRATION CHECK*
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = TOXL 8164.14.00 09/16
04/12/2021 13:03

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:03
02 Std. Gas	0.080	13:04
03 Room Air	0.000	13:04
04 Std. Gas	0.080	13:04
05 Room Air	0.000	13:05
06 Std. Gas	0.080	13:05
07 Room Air	0.000	13:06

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000