

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-005362

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 283 psi Regulator: 260 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2-13-22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12-8-22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3451 Lot #: ICS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 24119080A1 Cyl #: 6 Exp. Date: 11-5-21

Test 1	<u>0.080</u>	Test 4	<u>0.080</u>	Test 7	<u>0.080</u>
Test 2	<u>0.081</u>	Test 5	<u>0.080</u>	Test 8	<u>0.080</u>
Test 3	<u>0.080</u>	Test 6	<u>0.081</u>	Test 9	<u>0.080</u>
Average	<u>0.080</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ed.
Breath Analyst Signature

4-13-21
Date

Kali L. Niet
Reviewed by

4-17-2021
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = TOXL 8164.14.00 09/16
04/13/2021 13:37

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 6
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 05/22/2020
Slope 659
Intercept -620990

IR Calibration Date: 05/26/2020
 3um 9um

0th Coef(*100): -20883 -25370
1st Coef(*100): 265508 144960
2nd Coef(*100): 936 714
H2O adj(mg/l*10k): 391 379

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = TOXL 8164.14.00 09/16
04/13/2021 13:43

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:44
02 Std. Sol.	0.019	13:44
03 Room Air	0.000	13:45
04 Std. Sol.	0.020	13:46
05 Room Air	0.000	13:46
06 Std. Sol.	0.019	13:47
07 Room Air	0.000	13:47

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

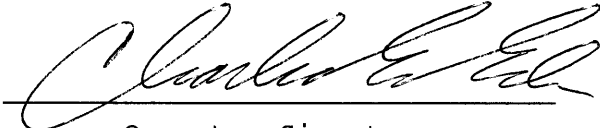

Operator Signature
CHARLES EDER

Remarks:

LOW AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = TOXL 8164.14.00 09/16
04/13/2021 13:49

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:49
02 Std. Sol.	0.300	13:50
03 Room Air	0.000	13:51
04 Std. Sol.	0.302	13:51
05 Room Air	0.000	13:52
06 Std. Sol.	0.301	13:53
07 Room Air	0.000	13:53

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: HIGH AC
 0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = TOXL 8164.14.00 09/16
04/13/2021 13:54

Test	AC	Time
01 Room Air	0.000	13:55
02 *Subject Test	INT*	13:55
03 Room Air	0.000	13:56

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 24119080A1
Cyl No = 6
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

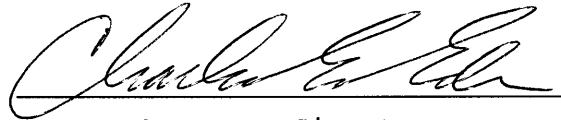

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = TOXL 8164.14.00 09/16
04/13/2021 13:56

Test	AC	Time
01 Diagnostic	OK	13:57
02 Room Air	0.000	13:58
03 *Subject Test	RFI*	13:58
04 Room Air	0.000	13:58

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 24119080A1
Cyl No = 6
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

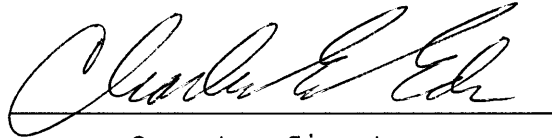

Operator Signature
CHARLES EDER

Remarks:



Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = TOXL 8164.14.00 09/16
04/13/2021 13:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:59
02 Std. Gas	0.080	13:59
03 Room Air	0.000	14:00
04 Std. Gas	0.081	14:00
05 Room Air	0.000	14:01
06 Std. Gas	0.080	14:01
07 Room Air	0.000	14:02

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *CALIBRATION CHECK*
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = TOXL 8164.14.00 09/16
04/13/2021 14:02

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:03
02 Std. Gas	0.080	14:03
03 Room Air	0.000	14:03
04 Std. Gas	0.080	14:04
05 Room Air	0.000	14:04
06 Std. Gas	0.081	14:05
07 Room Air	0.000	14:05

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = TOXL 8164.14.00 09/16
04/13/2021 14:05

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:06
02 Std. Gas	0.080	14:06
03 Room Air	0.000	14:07
04 Std. Gas	0.080	14:07
05 Room Air	0.000	14:08
06 Std. Gas	0.080	14:08
07 Room Air	0.000	14:09

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

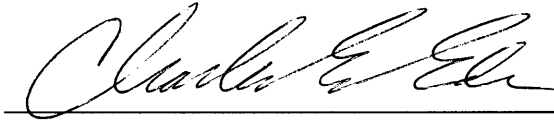

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
 0.080 AC

Form 106-I8000