

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004939

Location: TOXL

A. General Setup and Checks:

- 1. Diagnostic Tests Pass and Instrument in Ready Mode
- 2. Breath tube heated
- 3. Date, time and location code (Level 2,E). Re-set if necessary.
- 4. Print test (Level 1,P). Sign and attach test record.
- 5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 142 psi Regulator: 150 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP3057 Lot #: 20030 Exp. Date: 1.21.22

Configure dry gas standard for the following tests (Level 1,S).

- 2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS 6 Exp. Date: NA
 Display reads "Interferent Detect"
- 3. RFI Check (CMS Mode) Display reads "RFI Detect"
- 4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 24119080 A1 Cyl #: 6 Exp. Date: 11.5.21
Test 1 0.081 Test 4 0.082 Test 7 0.082
Test 2 0.081 Test 5 0.081 Test 8 0.081
Test 3 0.081 Test 6 0.082 Test 9 0.083
Average 0.082

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ed
Breath Analyst Signature

4.14.21
Date

Kali Y. Hib
Reviewed by

4-19-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.14.00 09/16
04/14/2021 16:08

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 6
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 01/18/2010
Slope 724
Intercept -779308

IR Calibration Date: 04/05/2017
 3um 9um

0th Coef(*100): -24406 -20805
1st Coef(*100): 261875 135290
2nd Coef(*100): 2828 1427
H2O adj(mg/l*10k): 563 393

***** Printer Test End *****

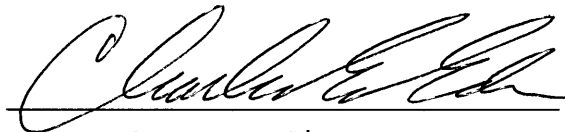

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.14.00 09/16
04/14/2021 16:09

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:10
02 Std. Sol.	0.020	16:10
03 Room Air	0.000	16:11
04 Std. Sol.	0.020	16:12
05 Room Air	0.000	16:12
06 Std. Sol.	0.020	16:13
07 Room Air	0.000	16:14

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

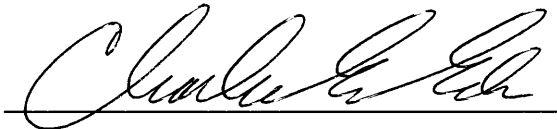

Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.14.00 09/16
04/14/2021 16:15

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:15
02 Std. Sol.	0.296	16:16
03 Room Air	0.000	16:17
04 Std. Sol.	0.296	16:17
05 Room Air	0.000	16:18
06 Std. Sol.	0.296	16:19
07 Room Air	0.000	16:19

08 Sim Temp = 34.0°C

Simul Ser No = MP3057
Std Sol No = 20030
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *HIGH AC*
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.14.00 09/16
04/14/2021 16:22

Test	AC	Time
01 Room Air	0.000	16:23
02 *Subject Test	INT*	16:23
03 Room Air	0.000	16:24

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 24119080A1
Cyl No = 6
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.14.00 09/16
04/14/2021 16:24

Test	AC	Time
01 Diagnostic	OK	16:24
02 Room Air	0.000	16:25
03 *Subject Test	RFI*	16:25
04 Room Air	0.000	16:26

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 24119080A1
Cyl No = 6
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.14.00 09/16
04/14/2021 16:26

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:26
02 Std. Gas	0.081	16:27
03 Room Air	0.000	16:27
04 Std. Gas	0.081	16:28
05 Room Air	0.000	16:28
06 Std. Gas	0.081	16:28
07 Room Air	0.000	16:29

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

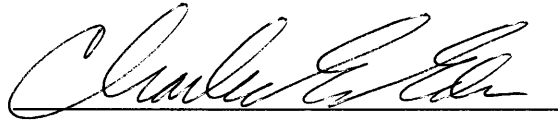

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.14.00 09/16
04/14/2021 16:29

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:30
02 Std. Gas	0.082	16:30
03 Room Air	0.000	16:31
04 Std. Gas	0.081	16:31
05 Room Air	0.000	16:31
06 Std. Gas	0.082	16:32
07 Room Air	0.000	16:32

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

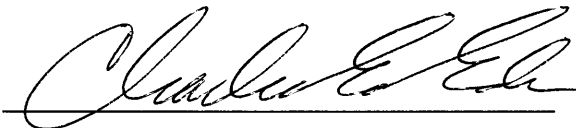

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.14.00 09/16
04/14/2021 16:32

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:33
02 Std. Gas	0.082	16:33
03 Room Air	0.000	16:34
04 Std. Gas	0.081	16:34
05 Room Air	0.000	16:35
06 Std. Gas	0.083	16:35
07 Room Air	0.000	16:36

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000