

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-003061

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 999 psi Regulator: 1000 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.015 AC
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.400 AC
Sim. Ser #: MP3060 Lot #: 1336 Exp. Date: 10-20-21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7348 Lot #: 1C55 Exp. Date: NA

Display reads "Interferent Detect"

3. RFI Check (CMS Mode) Display reads "RFI Detect"

4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC

Gas Cyl Lot #: 02621080A1 Cyl #: 0210 Exp. Date: 3-5-23

Test 1 0.078 Test 4 0.080 Test 7 0.079

Test 2 0.079 Test 5 0.080 Test 8 0.079

Test 3 0.080 Test 6 0.079 Test 9 0.079

Average 0.079

C. Remarks/Maintenance: Annual Inspection

Instrument is acceptable to be used in the field.

Kev L. Diet
Breath Analyst Signature

4-19-21
Date

Charles E. Egan
Reviewed by

4.19.21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003061
Location = TOXL 8164.14.00 09/16
04/19/2021 10:39

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 5
Standard Expiration? 02/05/2021
Oper No? 132598

Flow Cal. Date: 03/04/2011
Slope 700
Intercept -623726

IR Calibration Date: 04/10/2015
 3um 9um

0th Coef(*100): -25722 -17879
1st Coef(*100): 266163 136703
2nd Coef(*100): 2302 1151
H2O adj(mg/l*10k): 412 294

***** Printer Test End *****

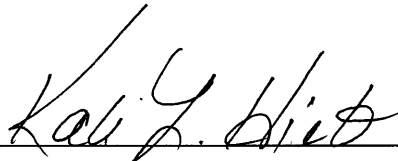

Operator Signature
KALI HIEB

Remarks: *print test*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003061
Location = TOXL 8164.14.00 09/16
04/19/2021 10:50

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:51
02 Std. Sol.	0.014	10:52
03 Room Air	0.000	10:52
04 Std. Sol.	0.013	10:53
05 Room Air	0.000	10:54
06 Std. Sol.	0.014	10:54
07 Room Air	0.000	10:55


08 Sim Temp = 34.0°C

Simul Ser No = MP5319

Std Sol No = 201911C

County = 08

Oper No. = 132598



Operator Signature

KALI HIEB

Remarks:

Cal check
Low AC 0.015

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003061
Location = TOXL 8164.14.00 09/16
04/19/2021 11:00

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:01
02 Std. Sol.	0.405	11:02
03 Room Air	0.000	11:02
04 Std. Sol.	0.408	11:03
05 Room Air	0.000	11:04
06 Std. Sol.	0.408	11:04
07 Room Air	0.000	11:05

08 Sim Temp = 34.0°C

Simul Ser No = MP3060
Std Sol No = ~~133L~~ 19108 KH
County = 08 Oper No. = 132598

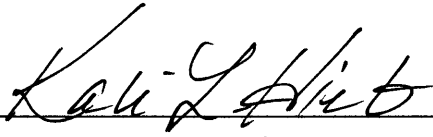

Operator Signature
KALI HIEB

Remarks: Cal check
 High AC 0.400
 Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003061
Location = TOXL 8164.14.00 09/16
04/19/2021 11:08

Test	AC	Time
01 Room Air	0.000	11:09
02 *Subject Test	INT*	11:10
03 Room Air	0.000	11:10

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

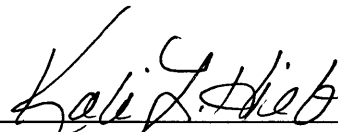

Operator Signature
KALI HIEB

Remarks: *Interferent*
0.10AC + 0.059% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003061
Location = TOXL 8164.14.00 09/16
04/19/2021 11:12

Test	AC	Time
01 Diagnostic	OK	11:13
02 Room Air	0.000	11:13
03 *Subject Test	RFI*	11:14
04 Room Air	0.000	11:14

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

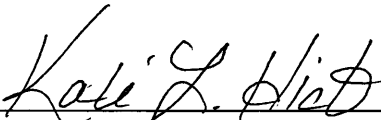

Operator Signature
KALI HIEB

Remarks: *RFI Check*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003061
Location = TOXL 8164.14.00 09/16
04/19/2021 11:15

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:16
02 Std. Gas	0.078	11:16
03 Room Air	0.000	11:17
04 Std. Gas	0.079	11:17
05 Room Air	0.000	11:17
06 Std. Gas	0.080	11:18
07 Room Air	0.000	11:18

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

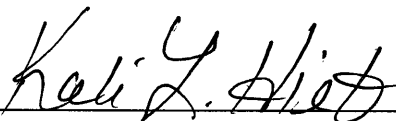

Operator Signature
KALI HIEB

Remarks: *cal check 0.080AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003061
Location = TOXL 8164.14.00 09/16
04/19/2021 11:19

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:19
02 Std. Gas	0.080	11:20
03 Room Air	0.000	11:20
04 Std. Gas	0.080	11:21
05 Room Air	0.000	11:21
06 Std. Gas	0.079	11:21
07 Room Air	0.000	11:22

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

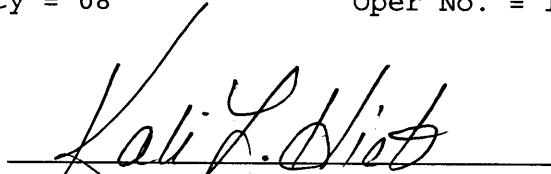
Operator Signature
KALI HIEB

Remarks:

Cal check 0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003061
Location = TOXL 8164.14.00 09/16
04/19/2021 11:24

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:24
02 Std. Gas	0.079	11:24
03 Room Air	0.000	11:25
04 Std. Gas	0.079	11:25
05 Room Air	0.000	11:26
06 Std. Gas	0.079	11:26
07 Room Air	0.000	11:27

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

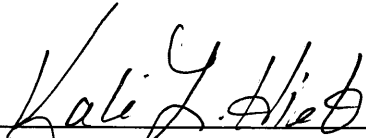

Operator Signature
KALI HIEB

Remarks: *Cal check O.DBD AC*

Form 106-I8000