

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-003071

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 947 psi Regulator: 950 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.015 AC
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11.19.21
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.400 AC
Sim. Ser #: MP3060 Lot #: 19108 Exp. Date: 10.20.21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR734B Lot #: 1C55 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot # 02L210B0A1 Cyl #: 26 Exp. Date: 3-5-23

Test 1 <u>0.078</u>	Test 4 <u>0.078</u>	Test 7 <u>0.079</u>
Test 2 <u>0.078</u>	Test 5 <u>0.079</u>	Test 8 <u>0.079</u>
Test 3 <u>0.078</u>	Test 6 <u>0.079</u>	Test 9 <u>0.078</u>
Average <u>0.078</u>		

C. Remarks/Maintenance: Annual Inspection
Replaced O-ring on simulator return.

Instrument is acceptable to be used in the field.

Kalip. Ditt
Breath Analyst Signature

4.20.21
Date

Charles E. Ed
Reviewed by

4.20.21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = TOXL 8164.14.00 09/16
04/20/2021 10:34

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 5
Standard Expiration? 02/05/2021
Oper No? 132598

Flow Cal. Date: 07/09/2010
Slope 806
Intercept -994737

IR Calibration Date: 04/10/2015
 3um 9um

	3um	9um
0th Coef(*100):	-11328	-10938
1st Coef(*100):	268087	134278
2nd Coef(*100):	3093	1368
H2O adj(mg/l*10k):	242	233

***** Printer Test End *****

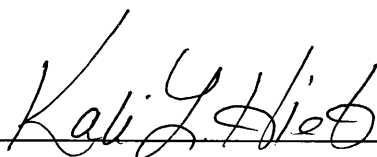

Operator Signature
KALI HIEB

Remarks:

Print test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = TOXL 8164.14.00 09/16
04/20/2021 10:40

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:41
02 Std. Sol.	0.014	10:43
03 Room Air	0.000	10:44
04 Std. Sol.	0.014	10:44
05 Room Air	0.000	10:45
06 Std. Sol.	0.014	10:46
07 Room Air	0.000	10:46

08 Sim Temp = 34.0°C

Simul Ser No = MP5319
Std Sol No = 201911C
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: *low AC 0.015*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = TOXL 8164.14.00 09/16
04/20/2021 10:47

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:48
02 Std. Sol.	0.408	10:49
03 Room Air	0.000	10:50
04 Std. Sol.	0.410	10:50
05 Room Air	0.000	10:51
06 Std. Sol.	0.411	10:52
07 Room Air	0.000	10:52

08 Sim Temp = 34.0°C

Simul Ser No = MP3060
Std Sol No = 19108
County = 08 Oper No. = 132598

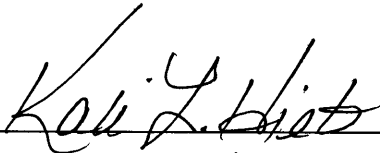

Operator Signature
KALI HIEB

Remarks: *High AC 0.400*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = TOXL 8164.14.00 09/16
04/20/2021 10:55

Test	AC	Time
01 Room Air	0.000	10:56
02 *Subject Test	INT*	10:57
03 Room Air	0.000	10:58

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

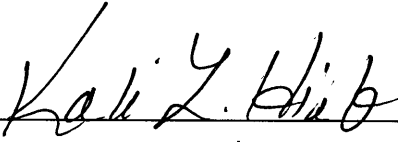

Operator Signature
KALI HIEB

Remarks: *Interferent Check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = TOXL 8164.14.00 09/16
04/20/2021 10:59

Test	AC	Time
01 Diagnostic	OK	11:00
02 Room Air	0.000	11:00
03 Reference	RFI*	11:00
04 Room Air	0.000	11:01

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

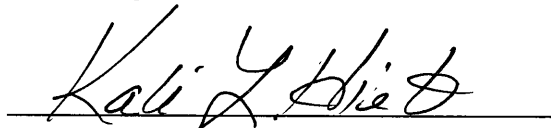

Operator Signature
KALI HIEB

Remarks:

RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = TOXL 8164.14.00 09/16
04/20/2021 11:01

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:02
02 Std. Gas	0.078	11:02
03 Room Air	0.000	11:03
04 Std. Gas	0.078	11:03
05 Room Air	0.000	11:03
06 Std. Gas	0.078	11:04
07 Room Air	0.000	11:04

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

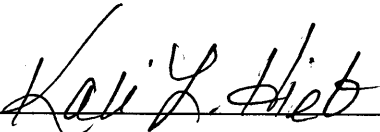

Operator Signature
KALI HIEB

Remarks: CAL CHECK 0.0BAC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = TOXL 8164.14.00 09/16
04/20/2021 11:05

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:05
02 Std. Gas	0.078	11:06
03 Room Air	0.000	11:06
04 Std. Gas	0.079	11:06
05 Room Air	0.000	11:07
06 Std. Gas	0.079	11:07
07 Room Air	0.000	11:08

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

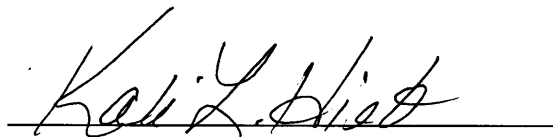
Operator Signature
KALI HIEB

Remarks:

CAL CHECK O.D.B.A.C

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = TOXL 8164.14.00 09/16
04/20/2021 11:09

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:09
02 Std. Gas	0.079	11:09
03 Room Air	0.000	11:10
04 Std. Gas	0.079	11:10
05 Room Air	0.000	11:11
06 Std. Gas	0.078	11:11
07 Room Air	0.000	11:12

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

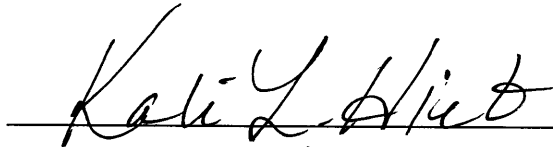
Operator Signature
KALI HIEB

Remarks: *cal check 0.000AC*

Form 106-I8000