

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004188

Location: TOLL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 968 psi Regulator: 950 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.019 AC  
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.400 AC  
Sim. Ser #: MP3060 Lot #: 1910B Exp. Date: 10-20-21

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR7348 Lot #: 1C55 Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 02621080A1 Cyl #: 026 Exp. Date: 3-5-23

Test 1 <u>0.078</u>	Test 4 <u>0.079</u>	Test 7 <u>0.079</u>
Test 2 <u>0.079</u>	Test 5 <u>0.079</u>	Test 8 <u>0.079</u>
Test 3 <u>0.079</u>	Test 6 <u>0.079</u>	Test 9 <u>0.079</u>
Average <u>0.079</u>		

C. Remarks/Maintenance:

Annual Inspection.  
Replaced O-ring on simulator return.

Instrument is acceptable to be used in the field.

Karl L. Hilt  
Breath Analyst Signature

04-20-21  
Date

Paul E. Ed  
Reviewed by

4.20.21  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004188  
Location = TOXL                8164.14.00 09/16  
04/20/2021                      15:27

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup


Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?         1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            34917080A3  
Standard Cyl #?            2  
Standard Expiration?       02/05/2020  
Oper No?                    132598

Flow Cal. Date:            04/30/2020  
Slope                      645  
Intercept                  -637424

IR Calibration Date:        05/06/2020

	3um	9um
0th Coef(*100):	-30092	-33449
1st Coef(*100):	293453	143538
2nd Coef(*100):	151	602
H2O adj(mg/l*10k):	425	462

\*\*\*\*\* Printer Test End \*\*\*\*\*

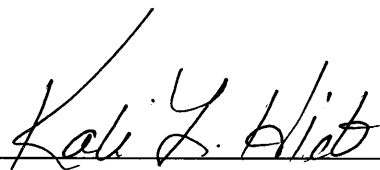

Operator Signature  
KALI HIEB

Remarks: *print test*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004188  
Location = TOXL                 8164.14.00 09/16  
04/20/2021                        15:30

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:30
02 Std. Sol.	0.014	15:32
03 Room Air	0.000	15:33
04 Std. Sol.	0.015	15:33
05 Room Air	0.000	15:34
06 Std. Sol.	0.015	15:35
07 Room Air	0.000	15:35

08 Sim Temp = 34.0°C

Simul Ser No = MP5319  
Std Sol No = 201911C  
County = 08                        Oper No. = 132598

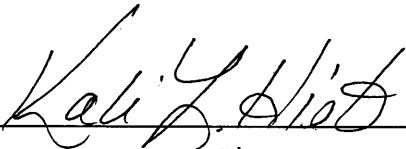  
\_\_\_\_\_  
Operator Signature  
KALI HIEB

Remarks: *Low AC 0.015*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004188  
Location = TOXL      8164.14.00 09/16  
04/20/2021      15:36

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:37
02 Std. Sol.	0.399	15:38
03 Room Air	0.000	15:38
04 Std. Sol.	0.402	15:39
05 Room Air	0.000	15:40
06 Std. Sol.	0.404	15:40
07 Room Air	0.000	15:41

08 Sim Temp = 33.9°C

Simul Ser No = MP3060  
Std Sol No = 19108  
County = 08      Oper No. = 132598

  
Operator Signature  
KALI HIEB

Remarks: *High AC 0.400*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004188  
Location = TOXL                    8164.14.00 09/16  
04/20/2021                            15:55

Test	AC	Time
01 Room Air	0.000	15:57
02 *Subject Test	INT*	15:57
03 Room Air	0.000	15:58

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 02621080A1  
Cyl No = 026  
Expiration Date = 03/05/2023  
County = 08                            Oper No. = 132598

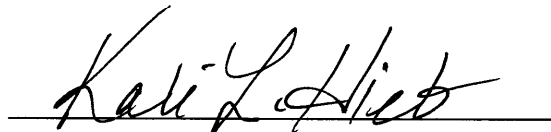

Operator Signature  
KALI HIEB

Remarks: *Interferent Check*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-004188  
Location = TOXL                              8164.14.00 09/16  
04/20/2021    16:00

Test	AC	Time
01 Diagnostic	OK	16:01
02 Room Air	0.000	16:01
03 Reference	RFI*	16:01
04 Room Air	0.000	16:02

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                              Weight = 150  
Test = DUI    Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 02621080A1  
Cyl No = 026  
Expiration Date = 03/05/2023  
County = 08                                      Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

  
Operator Signature  
KALI HIEB

Remarks: *RFI check*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004188  
Location = TOXL                    8164.14.00 09/16  
04/20/2021                            15:43

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:44
02 Std. Gas	0.078	15:44
03 Room Air	0.000	15:45
04 Std. Gas	0.079	15:45
05 Room Air	0.000	15:45
06 Std. Gas	0.079	15:46
07 Room Air	0.000	15:46

Lot No = 02621080A1  
Cyl No = 026  
Exp Date = 03/05/2023  
County = 08                            Oper No. = 132598

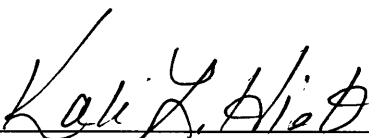  
\_\_\_\_\_  
Operator Signature  
KALI HIEB

Remarks: *cal check 0.080 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004188  
Location = TOXL      8164.14.00 09/16  
04/20/2021      15:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:47
02 Std. Gas	0.079	15:47
03 Room Air	0.000	15:48
04 Std. Gas	0.079	15:48
05 Room Air	0.000	15:49
06 Std. Gas	0.079	15:49
07 Room Air	0.000	15:50

Lot No = 02621080A1  
Cyl No = 026  
Exp Date = 03/05/2023  
County = 08      Oper No. = 132598

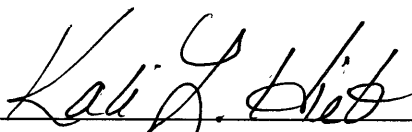

Operator Signature  
KALI HIEB

Remarks: *Cal Check 0.000 AC*

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004188  
Location = TOXL      8164.14.00 09/16  
04/20/2021      15:51

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:51
02 Std. Gas	0.079	15:52
03 Room Air	0.000	15:52
04 Std. Gas	0.079	15:52
05 Room Air	0.000	15:53
06 Std. Gas	0.079	15:53
07 Room Air	0.000	15:54

Lot No = 02621080A1  
Cyl No = 026  
Exp Date = 03/05/2023  
County = 08      Oper No. = 132598

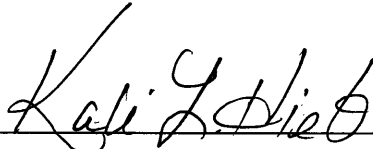  
\_\_\_\_\_  
Operator Signature  
KALI HIEB

Remarks: *cal check 0.000 AC*

Form 106-I8000