

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004196

Location: TOVL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 904 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value \leq 0.03 AC: 0.015 AC
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b. High AC (Level 1,C): Known Value \geq 0.25 AC: 0.400 AC
Sim. Ser #: MP3060 Lot #: 19108 Exp. Date: 10-20-21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: ^{VLT 0.10} 0.05 AC + 0.05% Acetone
Sim. Ser #: DR7349 Lot #: 1055 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 216 Exp. Date: 3-5-23

Test 1 <u>0.078</u>	Test 4 <u>0.078</u>	Test 7 <u>0.077</u>
Test 2 <u>0.078</u>	Test 5 <u>0.078</u>	Test 8 <u>0.077</u>
Test 3 <u>0.077</u>	Test 6 <u>0.078</u>	Test 9 <u>0.078</u>
Average <u>0.078</u>		

C. Remarks/Maintenance: Annual Inspection. Replaced O-ring on simulator return.

Instrument is acceptable to be used in the field.

Katya Shih
Breath Analyst Signature

04-27-21
Date

Charles E. Eh
Reviewed by

4.27.2021
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
04/27/2021 01:47

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 5
Standard Expiration? 02/05/2021
Oper No? 132598

Flow Cal. Date: 04/15/2020
Slope 657
Intercept -683120

IR Calibration Date: 04/16/2020
 3um 9um

0th Coef(*100): -35275 -26830
1st Coef(*100): 271852 134658
2nd Coef(*100): 1067 849
H2O adj(mg/l*10k): 413 302

***** Printer Test End *****

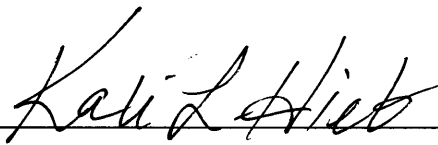

Operator Signature
KALI HIEB

Remarks: *print test*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
04/27/2021 01:51

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	01:52
02 Std. Sol.	0.012	01:53
03 Room Air	0.000	01:53
04 Std. Sol.	0.013	01:54
05 Room Air	0.000	01:54
06 Std. Sol.	0.013	01:55
07 Room Air	0.000	01:56

08 Sim Temp = 34.0°C

Simul Ser No = MP5319
Std Sol No = 201911C
County = 08 Oper No. = 132598

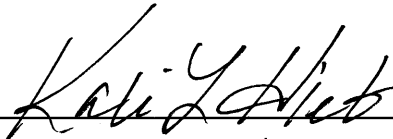

Operator Signature
KALI HIEB

Remarks: *Low AC Cal check*
0.015 AC
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
04/27/2021 04:06

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	04:07
02 Std. Sol.	0.411	04:08
03 Room Air	0.000	04:08
04 Std. Sol.	0.412	04:09
05 Room Air	0.000	04:09
06 Std. Sol.	0.411	04:10
07 Room Air	0.000	04:11

08 Sim Temp = 33.9°C

Simul Ser No = MP3060
Std Sol No = 19108
County = 08 Oper No. = 132598



Operator Signature
KALI HIEB

Remarks: High ac cal check
0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
04/27/2021 04:17

Test	AC	Time
01 Room Air	0.000	04:18
02 *Subject Test	INT*	04:19
03 Room Air	0.000	04:19

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

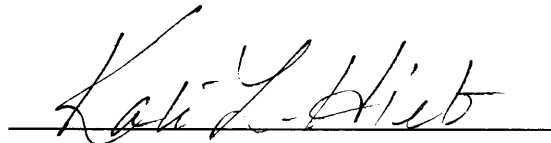

Operator Signature
KALI HIEB

Remarks: *Interferent Check*
0.104C + 0.059% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
04/27/2021 04:20

Test	AC	Time
01 Diagnostic	OK	04:21
02 Room Air	0.000	04:22
03 Reference	RFI*	04:22
04 Room Air	0.000	04:22

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

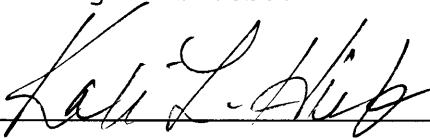

Operator Signature
KALI HIEB

Remarks: *RFI check*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
04/27/2021 04:23

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	04:24
02 Std. Gas	0.078	04:24
03 Room Air	0.000	04:25
04 Std. Gas	0.078	04:25
05 Room Air	0.000	04:26
06 Std. Gas	0.077	04:26
07 Room Air	0.000	04:27

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

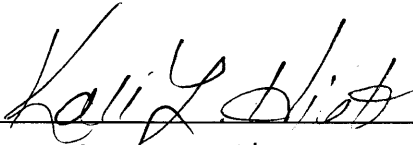

Operator Signature
KALI HIEB

Remarks: *Dry cal check 0.080AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
04/27/2021 04:27

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	04:28
02 Std. Gas	0.078	04:28
03 Room Air	0.000	04:29
04 Std. Gas	0.078	04:29
05 Room Air	0.000	04:30
06 Std. Gas	0.078	04:30
07 Room Air	0.000	04:31

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

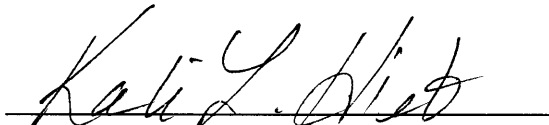
Operator Signature
KALI HIEB

Remarks: *Dry cal check 0.080 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
04/27/2021 04:31

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	04:32
02 Std. Gas	0.077	04:32
03 Room Air	0.000	04:33
04 Std. Gas	0.077	04:33
05 Room Air	0.000	04:34
06 Std. Gas	0.078	04:34
07 Room Air	0.000	04:34

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

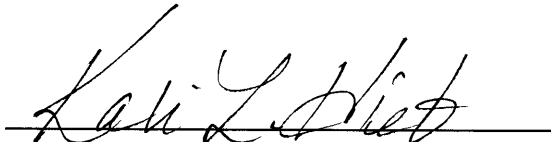
Operator Signature
KALI HIEB

Remarks: *Dry cal check 0.060 AC*

Form 106-I8000