

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004935

Location: TOXL

A. General Setup and Checks:

- 1. Diagnostic Tests Pass and Instrument in Ready Mode
- 2. Breath tube heated
- 3. Date, time and location code (Level 2,E). Re-set if necessary.
- 4. Print test (Level 1,P). Sign and attach test record.
- 5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 225 psi Regulator: 225 psi
CEE 232

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

- 1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

- 2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR5114 Lot #: ICSG Exp. Date: NA
- Display reads "Interferent Detect"
- 3. RFI Check (CMS Mode) Display reads "RFI Detect"
- 4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 05620080A1 Cyl #: 48 Exp. Date: 4.5.22

Test 1 <u>0.079</u>	Test 4 <u>0.079</u>	Test 7 <u>0.078</u>
Test 2 <u>0.078</u>	Test 5 <u>0.078</u>	Test 8 <u>0.077</u>
Test 3 <u>0.079</u>	Test 6 <u>0.078</u>	Test 9 <u>0.079</u>
Average <u>0.078</u>		

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles Lee
Breath Analyst Signature

21
4.28.22 CEE
Date

Kai L. Hib
Reviewed by

5.3.21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = TOXL 8164.14.00 09/16
04/28/2021 09:31

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 02621080A1
Standard Cyl #? 25
Standard Expiration? 03/05/2023
Oper No? 666666

Flow Cal. Date: 07/12/2012
Slope 655
Intercept -510289

IR Calibration Date: 05/20/2015
 3um 9um

0th Coef(*100): -7871 -19684
1st Coef(*100): 264505 133108
2nd Coef(*100): 2865 1320
H2O adj (mg/l*10k): 200 298

***** Printer Test End *****

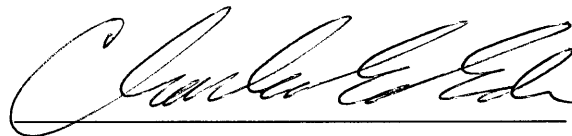

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = TOXL 8164.14.00 09/16
04/28/2021 09:33

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:34
02 Std. Sol.	0.019	09:34
03 Room Air	0.000	09:35
04 Std. Sol.	0.018	09:36
05 Room Air	0.000	09:36
06 Std. Sol.	0.019	09:37
07 Room Air	0.000	09:37

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = TOXL 8164.14.00 09/16
04/28/2021 09:39

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:40
02 Std. Sol.	0.300	09:41
03 Room Air	0.000	09:41
04 Std. Sol.	0.301	09:42
05 Room Air	0.000	09:43
06 Std. Sol.	0.300	09:43
07 Room Air	0.000	09:44

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

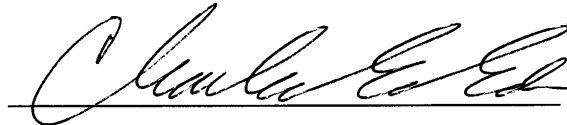

Operator Signature
CHARLES EDER

Remarks: HIGH AC
 0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = TOXL 8164.14.00 09/16
04/28/2021 09:46

Test	AC	Time
01 Room Air	0.000	09:47
02 *Subject Test	INT*	09:47
03 Room Air	0.000	09:48

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 05620080A1
Cyl No = 48
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

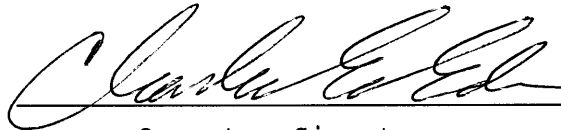

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = TOXL 8164.14.00 09/16
04/28/2021 09:49

Test	AC	Time
01 Diagnostic	OK	09:49
02 Room Air	0.000	09:50
03 *Subject Test	RFI*	09:50
04 Room Air	0.000	09:51

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 05620080A1
Cyl No = 48
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:



Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = TOXL 8164.14.00 09/16
04/28/2021 10:00

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:01
02 Std. Gas	0.079	10:01
03 Room Air	0.000	10:02
04 Std. Gas	0.078	10:02
05 Room Air	0.000	10:03
06 Std. Gas	0.079	10:03
07 Room Air	0.000	10:04

Lot No = 05620080A1
Cyl No = 48
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

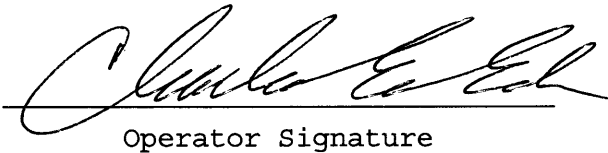

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = TOXL 8164.14.00 09/16
04/28/2021 10:04

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:04
02 Std. Gas	0.079	10:05
03 Room Air	0.000	10:05
04 Std. Gas	0.078	10:05
05 Room Air	0.000	10:06
06 Std. Gas	0.078	10:06
07 Room Air	0.000	10:07

Lot No = 05620080A1
Cyl No = 48
Exp Date = 04/05/2022
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = TOXL 8164.14.00 09/16
04/28/2021 10:07

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:08
02 Std. Gas	0.078	10:08
03 Room Air	0.000	10:09
04 Std. Gas	0.077	10:09
05 Room Air	0.000	10:09
06 Std. Gas	0.079	10:10
07 Room Air	0.000	10:10

Lot No = 05620080A1
Cyl No = 48
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

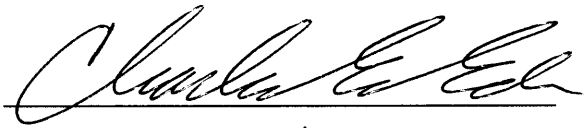

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000