

INTOXILYZER® 8000 INITIAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004194

A. GENERAL Setup and Checks:

- 1. Power On
 - 5 min. countdown during initial warm-up
 - 1 min. countdown to begin test after standby mode
- 2. Display Intensity (Ctrl + ↑ or ↓)
- 3. Password Security:
 - Level 1 (Operator) Level 2 (Field Inspector) Level 3 (Lab Personnel)
- 4. Printer Setup (Level 3,S,P)
- 5. Forms Load (CMI, Inc., CoBrA Software)

B. LEVEL 1 Setup and Checks:

- 1. Internal Printer Test and Paper Feed (Level 1,P). Attach record.
- 2. External Printer Test (Level 1,P). Attach record.
- 3. Barcode Reader (Level 1,B):
 - Operator ID ND License R key: Refusal. Attach record.

C. LEVEL 2 Setup and Checks:

- 1. Continuous Air Blank (Level 2,A)
- 2. Diagnostic (Level 2,D). Attach record.
- 3. Prelim Data Entry (Level 2,E)
- 4. Ser Number/Version Info (Level 2,V):
 - Inst Ser#: 80-004194 DSP Ver: 1362.14
 - Core Ver: 8164.14 CPLD Ver: 7

D. LEVEL 3 Setup and Checks:

- 1. DVM Monitor (Level 3,D,D): 3: 12338 s: 1 c: 47.00
9: 12332 s: 1 B: 45 0
(RFI indicator with keyed radio): 1
- 2. Function (F) Keys : F5 – Tone F9 - Fan
 F6 – Green LED F10 – Pump
 F7 – Red LED F11 – Solenoid
- 3. Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 954 CF: 1.06
- 4. Flow Monitor (Level 3,D,F): Flow Sensor, R: 192 F: 0.000 L/s

5. Temperature Monitor (Level 3,D,T): C: 47.0 A: 47.0 I: 0.0
B: 45.0 V: 0.0
6. Tank Monitor (Level 3,D,G): P (display): 231 psi P (gauge): 250 psi
7. General Setup (Level 3,S,G)
8. Configure Start Test (Level 3,S,T)
9. Network (Level 3,S,N)

E. TESTS (attach all test records):

Configure wet bath simulator standards before running tests (Level 1,S):

1. Zero AC (Level 1,C):
Sim ser #: MP5320 Lot #: MILLI Q H₂O Exp date: NA
Known value: 0.000 AC
Results: 0.000 AC 0.000 AC 0.000 AC
2. Low AC (Level 1,C):
Sim ser #: MP5289 Lot #: 201911E Exp date: 11.19.21
Known value: 0.030 AC
Results: 0.029 AC 0.030 AC 0.030 AC
3. High AC (Level 1,C):
Sim ser #: MP3062 Lot #: 202103E Exp date: 3.24.23
Known value: 0.400 AC
Results: 0.406 AC 0.406 AC 0.405 AC

Configure dry gas standard before running tests (Level 1,S):

4. Ethanol + 0.05% Acetone (Level 1,B):
Sim ser #: DR5114 Lot #: ICS 6 Exp date: NA
Known value: 0.10 AC + 0.05% ACETONE
 Display reads "Interferent Detect"
5. Acetone (Level 1,B):
Sim ser #: DR5188 Lot #: ACE1 Exp date: NA
Known value: 0.05% ACETONE
 Display reads "Interferent Detect"
6. Methanol (Level 1,B):
Sim ser #: DR5186 Lot #: MET3 Exp date: NA
Known value: 0.10% METHANOL
 Display reads "Interferent Detect"
7. Isopropanol (Level 1,B):
Sim ser #: DR5189 Lot #: IPA2 Exp date: NA
Known value: 0.10% ISOPROPANOL
 Display reads "Interferent Detect"

- 8. Ambient Fail (Level 1,B): Display and test record read correct.
- 9. Invalid Sample (Level 1,B): Display and test record read correct.
- 10. Sequence Aborted (Level 1,B): Display and test record read correct.
- 11. ABA (Level 1,B): Test record reads correct.
- 12. Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- 13. RFI Detected (B,C, or CMS mode): Display and test record read correct.
- 14. Tank Pressure Below Minimum (CMS mode): Display reads correct.
- 15. Deficient Samples (CMS mode): Display and test record read correct.
- 16. Improper Sample (CMS mode): Display and test record read correct.
- 17. Difference Too Great (CMS mode): Display and test record read correct.
- 18. CMS (CMS mode): Test record reads correct.
- 19. Stability Test (Level 3,T,S):

Ave: 0.0795 Std Dev: 0.0008 Rel Std Dev: 1.04%

Maintenance/Repairs/Notes: INITIAL INSPECTION DUE TO REPLACING
REAL TIME CLOCK BATTERY AND HAVING TO OPEN UP
INSTRUMENT TO PERFORM THE REPAIR.

REPLACED SIMULATOR RETURN O-RINGS

Instrument is acceptable to be used in the field.

Charles E. Ehr

Field Inspector's Signature

4-29-21

Date

Kali L. Hiett

Reviewed by

5-3-21

Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 12:43

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMNQP

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQPQRSTU

24 characters per line
abcdefghijklmnopqrstuwx
ABCDEFGHIJKLMNQPQRSTUWX

32 characters per line
abcdefghijklmnopqrstuwx123456
ABCDEFGHIJKLMNQPQRSTUWXYZ123456

42 characters per line
abcdefghijklmnopqrstuwx1234567890abcdef
ABCDEFGHIJKLMNQPQRSTUWXYZ1234567890ABCDEFGHI


Current Instrument Setup
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On MemFull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 5
Standard Expiration? 02/05/2021
Oper No? 666656

Flow Cal. Date: 06/23/2009
Slope 681
Intercept -622430

IR Calibration Date: 05/04/2016
3um 9um

0th Coef(*100):	-17808	-24119
1st Coef(*100):	263893	132021
2nd Coef(*100):	3080	1296
H2O adj(mg/l*10K):	403	519

***** Test End *****



Operator Signature
CHARLES EDER

Remarks: *INTERNAL
PRINT TEST*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 13:06

Test	AC	Time
01 Room Air	0.000	13:06
02 *Subject Test	REF*	13:07
03 Room Air	0.000	13:07

*Subject Test Refused

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = R KEY REFUSAL
Dr. Lic. = ND/TES989643
Lot No = 34418080A2
Cyl No = 5
Expiration Date = 02/05/2021
County = 08 Oper No. = 666666

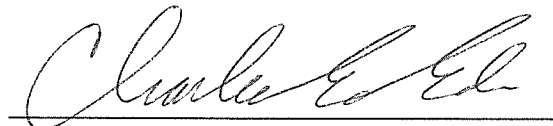

Operator Signature
CHARLES EDER

Remarks: "R" KEY REFUSAL

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 14:49

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:50
02 Std. Sol.	0.000	14:50
03 Room Air	0.000	14:51
04 Std. Sol.	0.000	14:52
05 Room Air	0.000	14:52
06 Std. Sol.	0.000	14:53
07 Room Air	0.000	14:53

08 Sim Temp = 34.0°C

Simul Ser No = MP5320
Std Sol No = MILLIQ H2O
County = 08 Oper No. = 666666

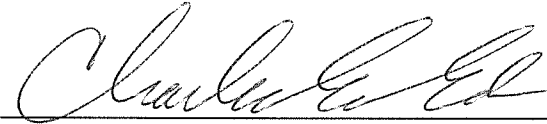

Operator Signature
CHARLES EDER

Remarks:

ZERO AC

0.000 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 14:54

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:55
02 Std. Sol.	0.029	14:56
03 Room Air	0.000	14:56
04 Std. Sol.	0.030	14:57
05 Room Air	0.000	14:58
06 Std. Sol.	0.030	14:58
07 Room Air	0.000	14:59

08 Sim Temp = 34.0°C

Simul Ser No = MP5289
Std Sol No = 201911E
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.030 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:00

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:00
02 Std. Sol.	0.406	15:01
03 Room Air	0.000	15:02
04 Std. Sol.	0.406	15:03
05 Room Air	0.000	15:03
06 Std. Sol.	0.405	15:04
07 Room Air	0.000	15:05

08 Sim Temp = 34.0°C

Simul Ser No = MP3062
Std Sol No = 202103E
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: HIGH AC
0.400 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:33

Test	AC	Time
01 Room Air	0.000	15:34
02 *Subject Test	INT*	15:34
03 Room Air	0.000	15:35

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10AC + 0.05% ACETONE

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:36

Test	AC	Time
01 Room Air	0.000	15:37
02 *Subject Test	INT*	15:37
03 Room Air	0.000	15:38

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.05% ACETONE

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:38

Test	AC	Time
01 Room Air	0.000	15:39
02 *Subject Test	INT*	15:39
03 Room Air	0.000	15:40

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

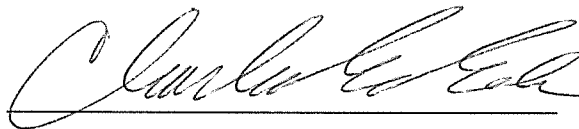

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10% METHANOL

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:41

Test	AC	Time
01 Room Air	0.000	15:42
02 *Subject Test	INT*	15:42
03 Room Air	0.000	15:43

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10% ISOPROPANOL

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:48

Test	AC	Time
01 Room Air	AMB*	15:49
02 Room Air	0.000	15:50

*Invalid Test
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = AMBIENT FAIL
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

AMBIENT FAIL

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:50

Test	AC	Time
01 Room Air	0.000	15:51
02 Invalid Sample	X.XXX	15:51
03 Room Air	0.000	15:52

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INVALID SAMPLE
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

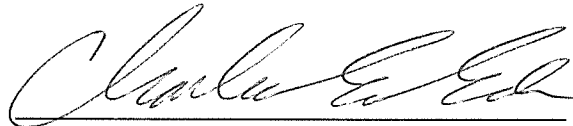

Operator Signature
CHARLES EDER

Remarks: *INVALID SAMPLE*
MOUTH ALCOHOL

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:53

Test	AC	Time
01 Room Air	0.000	15:54
02 *Subject Test	ABT*	15:54
03 Room Air	0.000	15:55

*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = SEQUENCE ABORT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: SEQUENCE ABORTED

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:55

Test	AC	Time
01 Room Air	0.000	15:56
02 Subject Test 1	0.147	15:56
03 Room Air	0.000	15:57
04 Reported AC	0.147	15:56

No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = ABA TEST
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

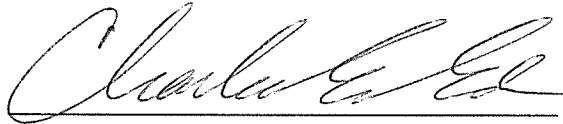

Operator Signature
CHARLES EDER

Remarks:

ABA TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 15:58

Test	AC	Time
01 Diagnostic	OK	15:58
02 Room Air	0.000	15:59
03 Subject Test 1	0.146	15:59
04 Room Air	0.000	16:02
05 Std. Gas	0.088*	16:03
06 Room Air	0.000	16:03

*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = CAL CHK OUT TOL
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
OUT OF TOLERANCE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 16:04

Test	AC	Time
01 Diagnostic	OK	16:05
02 Room Air	0.000	16:06
03 *Subject Test	RFI*	16:06
04 Room Air	0.000	16:06

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 16:07


Test	AC	Time
01 Diagnostic	OK	16:08
02 Room Air	0.000	16:09
03 *Subject Test	0.000*	16:12
04 Room Air	0.000	16:14
05 Std. Gas	0.080	16:15
06 Room Air	0.000	16:16
07 *Subject Test	0.000*	16:19
08 Room Air	0.000	16:20
No RFI Detected		

*Deficient Sample - Value Printed was
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = DEFICIENT SAMP
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.

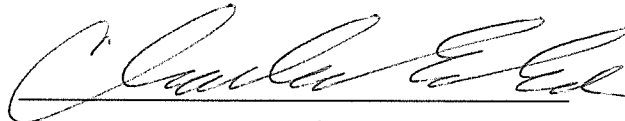

Operator Signature
CHARLES EDER

Remarks: DEFICIENT
SAMPLES

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 16:20

Test	AC	Time
01 Diagnostic	OK	16:21
02 Room Air	0.000	16:22
03 Reference	IPS*	16:22
04 Room Air	0.000	16:22

*Improper Sample

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = IMPROPER SAMPLE
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

*IMPROPER
SAMPLE*
Form 106-18000
CEE

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 16:23

Test	AC	Time
01 Diagnostic	OK	16:24
02 Room Air	0.000	16:25
03 Subject Test 1	0.197*	16:25
04 Room Air	0.000	16:27
05 Std. Gas	0.080	16:28
06 Room Air	0.000	16:30
07 Subject Test 2	0.145*	16:30
08 Room Air	0.000	16:31

*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = DIFF TOO GREAT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

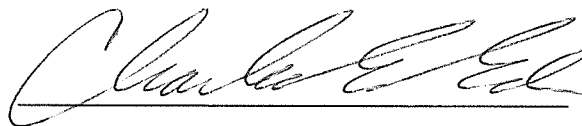

Operator Signature
CHARLES EDER

Remarks: *DIFFERENCE
TOO GREAT*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 16:32

Test	AC	Time
01 Diagnostic	OK	16:33
02 Room Air	0.000	16:33
03 Subject Test 1	0.145	16:34
04 Room Air	0.000	16:36
05 Std. Gas	0.078	16:37
06 Room Air	0.000	16:38
07 Subject Test 2	0.144	16:39
08 Room Air	0.000	16:40
09 Reported AC	0.144	16:39

Difference OK
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = CMS TEST
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

CMS TEST
CEE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004194
Location = TOXL 8164.14.00 09/16
04/29/2021 16:40

Test	AC	Time
01 Room Air	0.000	16:41
02 Std. Gas	0.078	16:41
03 Room Air	0.000	16:42
04 Std. Gas	0.078	16:42
05 Room Air	0.000	16:43
06 Std. Gas	0.080	16:43
07 Room Air	0.000	16:44
08 Std. Gas	0.079	16:44
09 Room Air	0.000	16:45
10 Std. Gas	0.079	16:45
11 Room Air	0.000	16:45
12 Std. Gas	0.079	16:46
13 Room Air	0.000	16:46
14 Std. Gas	0.080	16:47
15 Room Air	0.000	16:47
16 Std. Gas	0.079	16:48
17 Room Air	0.000	16:48
18 Std. Gas	0.079	16:48
19 Room Air	0.000	16:49
20 Std. Gas	0.080	16:49
21 Room Air	0.000	16:50
22 Std. Gas	0.079	16:50
23 Room Air	0.000	16:51
24 Std. Gas	0.079	16:51
25 Room Air	0.000	16:52
26 Std. Gas	0.079	16:52
27 Room Air	0.000	16:53
28 Std. Gas	0.079	16:53
29 Room Air	0.000	16:53
30 Std. Gas	0.081	16:54
31 Room Air	0.000	16:54
32 Std. Gas	0.080	16:55
33 Room Air	0.000	16:55
34 Std. Gas	0.080	16:56
35 Room Air	0.000	16:56
36 Std. Gas	0.080	16:56
37 Room Air	0.000	16:57
38 Std. Gas	0.081	16:57
39 Room Air	0.000	16:58
40 Std. Gas	0.080	16:58
41 Room Air	0.000	16:59
42 Cal Check Stats:		
43 Average	0.0795	
44 Std Dev	0.0008	
45 Rel Std Dev	1.04%	



Operator Signature
CHARLES EDER

Remarks:

0.080 AC
STABILITY TEST

Form 106-I8000

LOT: 02621 080 A 1

EXP: 3.5.23

CYL: 25