

**INTOXILYZER® 8000 INSPECTION**

Intoxilyzer® 8000 Serial Number: 80-005956

Location: TOXL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 864 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.015 AC  
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.400 AC  
Sim. Ser #: MP3060 Lot #: 1910B Exp. Date: 10-20-21

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR734B Lot #: 1C55 Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 026210B0A1 Cyl #: 0210 Exp. Date: 3-9-23

|                      |                     |                     |
|----------------------|---------------------|---------------------|
| Test 1 <u>0.078</u>  | Test 4 <u>0.078</u> | Test 7 <u>0.078</u> |
| Test 2 <u>0.078</u>  | Test 5 <u>0.079</u> | Test 8 <u>0.078</u> |
| Test 3 <u>0.077</u>  | Test 6 <u>0.078</u> | Test 9 <u>0.079</u> |
| Average <u>0.078</u> |                     |                     |

C. Remarks/Maintenance: Annual Inspection

Instrument is acceptable to be used in the field.

Kari L. Hiest  
Breath Analyst Signature

5.3.21  
Date

Charles E. Ehl  
Reviewed by

5.3.21  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005956  
Location = TOXL                    8164.14.00 09/16  
05/03/2021                            10:36

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

Current Instrument Setup


Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            05620080A1  
Standard Cyl #?            36  
Standard Expiration?       04/05/2022  
Oper No?                    132598

Flow Cal. Date:            06/21/2013  
Slope                        706  
Intercept                   -720901

IR Calibration Date:        04/02/2015

|                    | 3um    | 9um    |
|--------------------|--------|--------|
| 0th Coef(*100):    | -23934 | -22166 |
| 1st Coef(*100):    | 279293 | 133410 |
| 2nd Coef(*100):    | 3061   | 1559   |
| H2O adj(mg/l*10k): | 483    | 423    |

\*\*\*\*\* Printer Test End \*\*\*\*\*

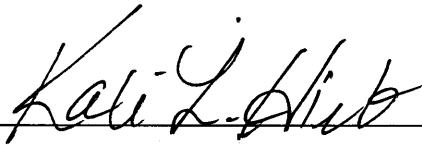  
\_\_\_\_\_  
Operator Signature  
KALI HIEB

Remarks: *print test*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005956  
Location = TOXL                    8164.14.00 09/16  
05/03/2021                            10:40

WET CAL CHECK

| Test         | AC    | Time  |
|--------------|-------|-------|
| 01 Room Air  | 0.000 | 10:41 |
| 02 Std. Sol. | 0.013 | 10:41 |
| 03 Room Air  | 0.000 | 10:42 |
| 04 Std. Sol. | 0.014 | 10:43 |
| 05 Room Air  | 0.000 | 10:43 |
| 06 Std. Sol. | 0.014 | 10:44 |
| 07 Room Air  | 0.000 | 10:44 |

08 Sim Temp = 34.0°C

Simul Ser No = MP5319  
Std Sol No = 201911C  
County = 08                            Oper No. = 132598

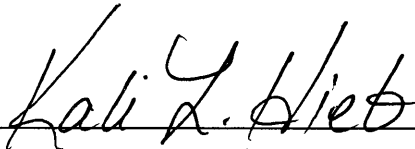

Operator Signature  
KALI HIEB

Remarks: *Low cal check 0.015 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005956  
Location = TOXL      8164.14.00 09/16  
05/03/2021      10:46

WET CAL CHECK

| Test         | AC    | Time  |
|--------------|-------|-------|
| 01 Room Air  | 0.000 | 10:47 |
| 02 Std. Sol. | 0.416 | 10:49 |
| 03 Room Air  | 0.000 | 10:49 |
| 04 Std. Sol. | 0.418 | 10:50 |
| 05 Room Air  | 0.000 | 10:50 |
| 06 Std. Sol. | 0.417 | 10:51 |
| 07 Room Air  | 0.000 | 10:52 |

08 Sim Temp = 33.9°C

Simul Ser No = MP3060  
Std Sol No = 19108  
County = 08      Oper No. = 132598



Operator Signature  
KALI HIEB

Remarks: *High cal check 0.400 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005956  
Location = TOXL                    8164.14.00 09/16  
05/03/2021                            10:56

| Test             | AC    | Time  |
|------------------|-------|-------|
| 01 Room Air      | 0.000 | 10:57 |
| 02 *Subject Test | INT*  | 10:57 |
| 03 Room Air      | 0.000 | 10:58 |

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 02621080A1  
Cyl No = 026  
Expiration Date = 03/05/2023  
County = 08                            Oper No. = 132598

  
\_\_\_\_\_  
Operator Signature  
KALI HIEB

Remarks: *Interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005956  
Location = TOXL                8164.14.00 09/16  
05/03/2021                        10:58

| Test          | AC    | Time  |
|---------------|-------|-------|
| 01 Diagnostic | OK    | 10:59 |
| 02 Room Air   | RFI*  | 11:00 |
| 03 Room Air   | 0.000 | 11:00 |

\*Invalid Test  
  Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                Weight = 150  
Test = DUI                        Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 02621080A1  
Cyl No = 026  
Expiration Date = 03/05/2023  
County = 08                        Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

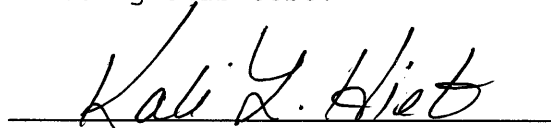

Operator Signature  
KALI HIEB

Remarks: *RFI check*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005956  
Location = TOXL      8164.14.00 09/16  
05/03/2021      11:01

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 11:02 |
| 02 Std. Gas | 0.078 | 11:02 |
| 03 Room Air | 0.000 | 11:03 |
| 04 Std. Gas | 0.078 | 11:03 |
| 05 Room Air | 0.000 | 11:04 |
| 06 Std. Gas | 0.077 | 11:04 |
| 07 Room Air | 0.000 | 11:04 |

Lot No = 02621080A1  
Cyl No = 026  
Exp Date = 03/05/2023  
County = 08      Oper No. = 132598

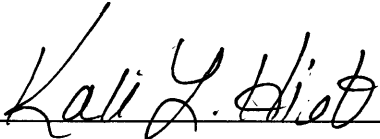  
\_\_\_\_\_  
Operator Signature  
KALI HIEB

Remarks: *cal check 0.000 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005956  
Location = TOXL      8164.14.00 09/16  
05/03/2021      11:05

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 11:06 |
| 02 Std. Gas | 0.078 | 11:06 |
| 03 Room Air | 0.000 | 11:07 |
| 04 Std. Gas | 0.079 | 11:07 |
| 05 Room Air | 0.000 | 11:08 |
| 06 Std. Gas | 0.078 | 11:08 |
| 07 Room Air | 0.000 | 11:09 |

Lot No = 02621080A1  
Cyl No = 026  
Exp Date = 03/05/2023  
County = 08      Oper No. = 132598

  
Operator Signature  
KALI HIEB

Remarks: *Cal check 0.000 AC*

Form 106-I8000



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005956  
Location = TOXL      8164.14.00 09/16  
05/03/2021      11:09

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 11:10 |
| 02 Std. Gas | 0.078 | 11:10 |
| 03 Room Air | 0.000 | 11:11 |
| 04 Std. Gas | 0.078 | 11:11 |
| 05 Room Air | 0.000 | 11:12 |
| 06 Std. Gas | 0.079 | 11:12 |
| 07 Room Air | 0.000 | 11:13 |

Lot No = 02621080A1  
Cyl No = 026  
Exp Date = 03/05/2023  
County = 08      Oper No. = 132598

  
Operator Signature  
KALI HIEB

Remarks: *cal check 0.080 AC*

Form 106-I8000