

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-005957

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 223 psi Regulator: 250 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02624080 A1 Cyl #: 25 Exp. Date: 3.5.23

Test 1 <u>0.079</u>	Test 4 <u>0.079</u>	Test 7 <u>0.079</u>
Test 2 <u>0.079</u>	Test 5 <u>0.079</u>	Test 8 <u>0.080</u>
Test 3 <u>0.079</u>	Test 6 <u>0.080</u>	Test 9 <u>0.079</u>
Average <u>0.079</u>		

C. Remarks/Maintenance: ANNUAL INSPECTION, TANK SENSOR CAL

Instrument is acceptable to be used in the field.

Charles E. Ed
Breath Analyst Signature

5.4.2021
Date

Kelli G. Hieb
Reviewed by

5-4-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005957
Location = TOXL 8164.14.00 09/16
05/04/2021 09:20

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%\$^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%\$^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 02621080A1
Standard Cyl #? 25
Standard Expiration? 03/05/2023
Oper No? 666666

Flow Cal. Date: 06/21/2013
Slope 647
Intercept -613317

IR Calibration Date: 05/11/2015

	3um	9um
0th Coef(*100):	-16666	-18045
1st Coef(*100):	278478	132949
2nd Coef(*100):	3303	1397
H2O adj(mg/l*10k):	379	351

***** Printer Test End *****

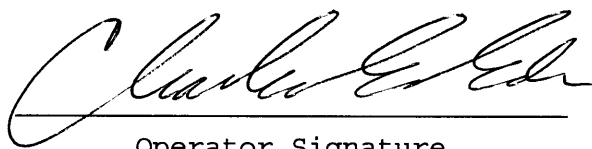

Operator Signature
CHARLES EDER

Remarks: PRINT TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005957
Location = TOXL 8164.14.00 09/16
05/04/2021 09:26

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:26
02 Std. Sol.	0.019	09:27
03 Room Air	0.000	09:28
04 Std. Sol.	0.018	09:28
05 Room Air	0.000	09:29
06 Std. Sol.	0.019	09:30
07 Room Air	0.000	09:30

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

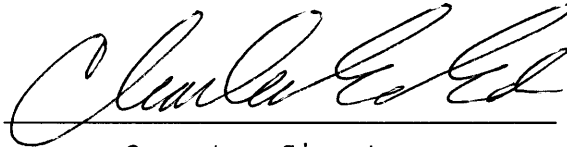

Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005957
Location = TOXL 8164.14.00 09/16
05/04/2021 09:31

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:32
02 Std. Sol.	0.296	09:32
03 Room Air	0.000	09:33
04 Std. Sol.	0.297	09:34
05 Room Air	0.000	09:34
06 Std. Sol.	0.297	09:35
07 Room Air	0.000	09:35

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

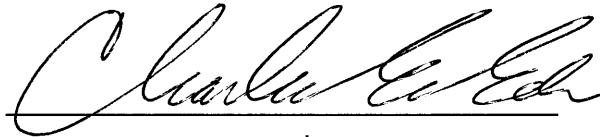

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005957
Location = TOXL 8164.14.00 09/16
05/04/2021 09:37

Test	AC	Time
01 Room Air	0.000	09:38
02 *Subject Test	INT*	09:39
03 Room Air	0.000	09:40

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

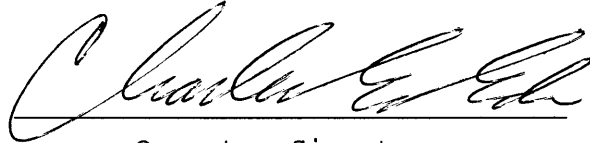

Operator Signature
CHARLES EDER

Remarks: ~~INT~~ INTERFERENT CHECK
CEE 0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005957
Location = TOXL 8164.14.00 09/16
05/04/2021 09:40

Test	AC	Time
01 Diagnostic	OK	09:41
02 Room Air	0.000	09:41
03 *Subject Test	RFI*	09:41
04 Room Air	0.000	09:42

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

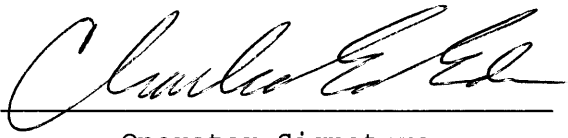

Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005957
Location = TOXL 8164.14.00 09/16
05/04/2021 09:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:43
02 Std. Gas	0.079	09:43
03 Room Air	0.000	09:43
04 Std. Gas	0.079	09:44
05 Room Air	0.000	09:44
06 Std. Gas	0.079	09:45
07 Room Air	0.000	09:45

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

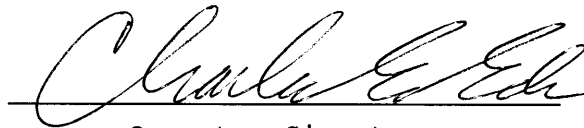

Operator Signature
CHARLES EDER

Remarks: *CALIBRATION CHECK*
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005957
Location = TOXL 8164.14.00 09/16
05/04/2021 09:45

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:46
02 Std. Gas	0.079	09:46
03 Room Air	0.000	09:47
04 Std. Gas	0.079	09:47
05 Room Air	0.000	09:48
06 Std. Gas	0.080	09:48
07 Room Air	0.000	09:49

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

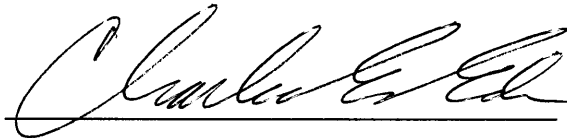

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC
Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005957
Location = TOXL 8164.14.00 09/16
05/04/2021 09:49

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:50
02 Std. Gas	0.079	09:50
03 Room Air	0.000	09:50
04 Std. Gas	0.080	09:51
05 Room Air	0.000	09:51
06 Std. Gas	0.079	09:52
07 Room Air	0.000	09:52

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

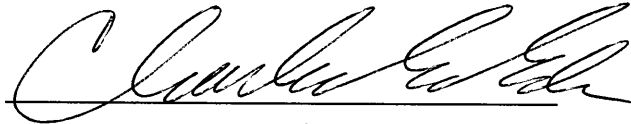

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000