

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004940

Location: TOHL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 854 psi Regulator: 850 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.015 AC
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.400 AC
Sim. Ser #: MP3060 Lot #: 19108 Exp. Date: 10-20-21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR734B Lot #: 1C55 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621086A1 Cyl #: 210 Exp. Date: 3-5-23

Test 1 <u>0.080</u>	Test 4 <u>0.079</u>	Test 7 <u>0.080</u>
Test 2 <u>0.080</u>	Test 5 <u>0.079</u>	Test 8 <u>0.080</u>
Test 3 <u>0.081</u>	Test 6 <u>0.081</u>	Test 9 <u>0.080</u>
Average <u>0.080</u>		

C. Remarks/Maintenance: Annual Inspection

Replaced breath hose, replaced external battery.

Instrument is acceptable to be used in the field.

Kate L. Hib
Breath Analyst Signature

5-4-21
Date

Charles E. Lee
Reviewed by

5-4-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004940
Location = TOXL 8164.14.00 09/16
05/04/2021 09:23

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 16
Standard Expiration? 11/05/2021
Oper No? 132598

Flow Cal. Date: 04/06/2020
Slope 635
Intercept -585462

IR Calibration Date: 04/06/2020

	3um	9um
0th Coef(*100):	-17993	-22378
1st Coef(*100):	260246	135868
2nd Coef(*100):	2982	1272
H2O adj(mg/l*10k):	383	361

***** Printer Test End *****

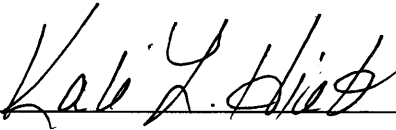

Operator Signature
KALI HIEB

Remarks: *print test*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004940
Location = TOXL 8164.14.00 09/16
05/04/2021 09:45

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:46
02 Std. Sol.	0.015	09:47
03 Room Air	0.000	09:47
04 Std. Sol.	0.014	09:48
05 Room Air	0.000	09:48
06 Std. Sol.	0.015	09:49
07 Room Air	0.000	09:50

08 Sim Temp = 34.0°C

Simul Ser No = MP5319
Std Sol No = 201911C
County = 08 Oper No. = 132598

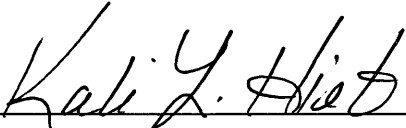

Operator Signature
KALI HIEB

Remarks: *low AC cal check 0.015AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004940
Location = TOXL 8164.14.00 09/16
05/04/2021 09:56

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:57
02 Std. Sol.	0.400	09:58
03 Room Air	0.000	09:58
04 Std. Sol.	0.409	09:59
05 Room Air	0.000	10:00
06 Std. Sol.	0.406	10:00
07 Room Air	0.000	10:01

08 Sim Temp = 33.9°C

Simul Ser No = MP3060
Std Sol No = 19108
County = 08 Oper No. = 132598

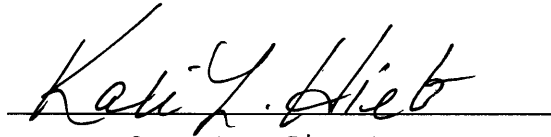

Operator Signature
KALI HIEB

Remarks: *low cal check*
High 0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004940
Location = TOXL 8164.14.00 09/16
05/04/2021 10:23

Test	AC	Time
01 Room Air	0.000	10:24
02 *Subject Test	INT*	10:24
03 Room Air	0.000	10:25

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

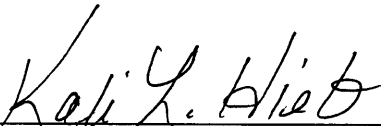

Operator Signature
KALI HIEB

Remarks: *Interferent Check*
0.1DAC + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004940
Location = TOXL 8164.14.00 09/16
05/04/2021 10:26

Test	AC	Time
01 Diagnostic	OK	10:27
02 Room Air	0.000	10:28
03 Reference	RFI*	10:28
04 Room Air	0.000	10:28

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

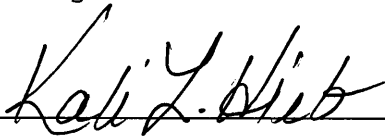

Operator Signature
KALI HIEB

Remarks: *RFI Check*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004940
Location = TOXL 8164.14.00 09/16
05/04/2021 14:07

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:08
02 Std. Gas	0.080	14:08
03 Room Air	0.000	14:09
04 Std. Gas	0.080	14:09
05 Room Air	0.000	14:09
06 Std. Gas	0.081	14:10
07 Room Air	0.000	14:10

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

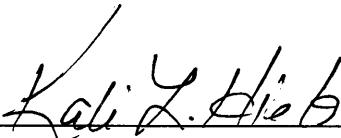

Operator Signature
KALI HIEB

Remarks: *cal check 0.080 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004940
Location = TOXL 8164.14.00 09/16
05/04/2021 14:11

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:11
02 Std. Gas	0.079	14:11
03 Room Air	0.000	14:12
04 Std. Gas	0.079	14:12
05 Room Air	0.000	14:13
06 Std. Gas	0.081	14:13
07 Room Air	0.000	14:14

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

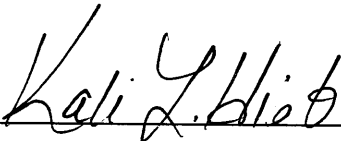

Operator Signature
KALI HIEB

Remarks: *cal check 0.000 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004940
Location = TOXL 8164.14.00 09/16
05/04/2021 14:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:14
02 Std. Gas	0.080	14:15
03 Room Air	0.000	14:15
04 Std. Gas	0.080	14:16
05 Room Air	0.000	14:16
06 Std. Gas	0.080	14:16
07 Room Air	0.000	14:17

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

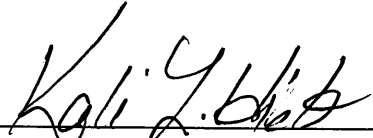

Operator Signature
KALI HIEB

Remarks: *cal check 0.080 AC*

Form 106-I8000