

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-005361

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 756 psi Regulator: 760 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.015 AC
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.400 AC
Sim. Ser #: MP3060 Lot #: 1910B Exp. Date: 10-20-21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR734B Lot #: 1C55 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 26 Exp. Date: 3-5-23

Test 1 <u>0.082</u>	Test 4 <u>0.080</u>	Test 7 <u>0.081</u>
Test 2 <u>0.081</u>	Test 5 <u>0.081</u>	Test 8 <u>0.081</u>
Test 3 <u>0.080</u>	Test 6 <u>0.080</u>	Test 9 <u>0.081</u>
Average <u>0.081</u>		

C. Remarks/Maintenance: Annual Inspection.

Replaced external battery.
Replaced simulator return O-ring and breath hose
O-ring. Replaced outlet hose connector.

Instrument is acceptable to be used in the field.

Kali Z. Hleb
Breath Analyst Signature

5-11-21
Date

Charles E. El
Reviewed by

5-17-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005361
Location = TOXL 8164.14.00 09/16
05/11/2021 09:36

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

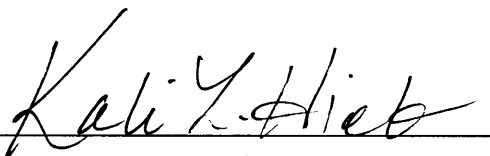
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 56
Standard Expiration? 02/05/2021
Oper No? 132598

Flow Cal. Date: 05/15/2020
Slope 634
Intercept -488053

IR Calibration Date: 05/15/2020

	3um	9um
0th Coef(*100):	-25383	-27323
1st Coef(*100):	288661	141732
2nd Coef(*100):	458	822
H2O adj(mg/l*10k):	335	405

***** Printer Test End *****


Operator Signature
KALI HIEB

Remarks: print test

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005361
Location = TOXL 8164.14.00 09/16
05/11/2021 10:00

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:01
02 Std. Sol.	0.014	10:02
03 Room Air	0.000	10:03
04 Std. Sol.	0.014	10:03
05 Room Air	0.000	10:04
06 Std. Sol.	0.014	10:05
07 Room Air	0.000	10:05

08 Sim Temp = 34.0°C

Simul Ser No = MP5319
Std Sol No = 201911C
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: *low AC 0.015 AC
check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005361
Location = TOXL 8164.14.00 09/16
05/11/2021 10:09

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:09
02 Std. Sol.	0.402	10:10
03 Room Air	0.000	10:11
04 Std. Sol.	0.406	10:11
05 Room Air	0.000	10:12
06 Std. Sol.	0.406	10:13
07 Room Air	0.000	10:13

08 Sim Temp = 33.9°C

Simul Ser No = MP3060
Std Sol No = 19108
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: High ac check 0.400 ac

Form 106-I8000

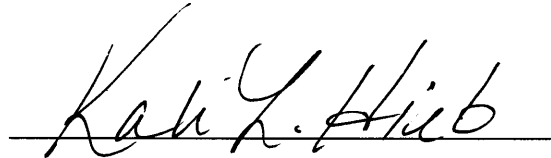
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005361
Location = TOXL 8164.14.00 09/16
05/11/2021 10:19

Test	AC	Time
01 Room Air	0.000	10:20
02 *Subject Test	INT*	10:21
03 Room Air	0.000	10:21

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: *Interferent Check*
0.10 AC + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

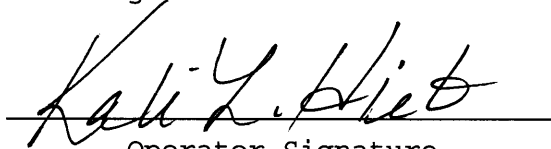
CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005361
Location = TOXL 8164.14.00 09/16
05/11/2021 11:05

Test	AC	Time
01 Diagnostic	OK	11:06
02 Room Air	0.000	11:07
03 Reference	RFI*	11:07
04 Room Air	0.000	11:07

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.


Operator Signature
KALI HIEB

Remarks: *RFI check*

Form 106-I8000

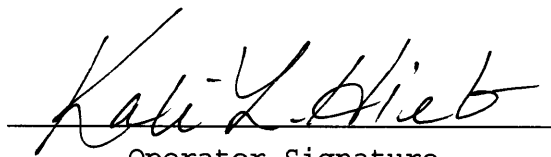
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005361
Location = TOXL 8164.14.00 09/16
05/11/2021 11:12

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:12
02 Std. Gas	0.082	11:13
03 Room Air	0.000	11:13
04 Std. Gas	0.081	11:14
05 Room Air	0.000	11:14
06 Std. Gas	0.080	11:15
07 Room Air	0.000	11:15

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: *Cal check 0.082AC*

Form 106-I8000

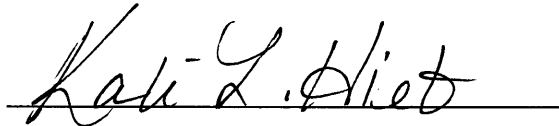
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005361
Location = TOXL 8164.14.00 09/16
05/11/2021 11:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:17
02 Std. Gas	0.080	11:17
03 Room Air	0.000	11:18
04 Std. Gas	0.081	11:18
05 Room Air	0.000	11:18
06 Std. Gas	0.080	11:19
07 Room Air	0.000	11:19

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: *cal check v. OBD AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005361
Location = TOXL 8164.14.00 09/16
05/11/2021 11:20

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:21
02 Std. Gas	0.081	11:21
03 Room Air	0.000	11:22
04 Std. Gas	0.081	11:22
05 Room Air	0.000	11:23
06 Std. Gas	0.081	11:23
07 Room Air	0.000	11:24

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: *Cal check O.OBAC*

Form 106-I8000