

**INTOXILYZER® 8000 INSPECTION**

Intoxilyzer® 8000 Serial Number: 80-004184 Location: TOXL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 222 psi Regulator: 250 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
  - a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.020 AC  
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
  - b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.300 AC  
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR3847 Lot #: FCS6 Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 02621080A1 Cyl #: 25 Exp. Date: 3.5.23

Test 1	<u>0.079</u>	Test 4	<u>0.078</u>	Test 7	<u>0.079</u>
Test 2	<u>0.079</u>	Test 5	<u>0.079</u>	Test 8	<u>0.079</u>
Test 3	<u>0.079</u>	Test 6	<u>0.079</u>	Test 9	<u>0.079</u>
Average	<u>0.079</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED EXTERNAL BATTERY

Instrument is acceptable to be used in the field.

Breath Analyst Signature

Reviewed by

Date

Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004184  
Location = TOXL                 8164.14.00 09/16  
05/17/2021                        08:52

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup


Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            24119080A1  
Standard Cyl #?            32  
Standard Expiration?       11/05/2021  
Oper No?                    666666

Flow Cal. Date:            07/30/2010  
Slope                      804  
Intercept                  -925008

IR Calibration Date:       12/07/2015  
                                    3um                      9um

-----  
0th Coef(\*100):           -15679                      -18680  
1st Coef(\*100):           263558                      136948  
2nd Coef(\*100):           2594                        1146  
H2O adj(mg/l\*10k):       405                         327

\*\*\*\*\* Printer Test End \*\*\*\*\*

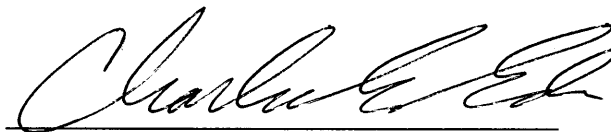

Operator Signature

CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004184  
Location = TOXL                    8164.14.00 09/16  
05/17/2021                            09:22

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:22
02 Std. Sol.	0.020	09:23
03 Room Air	0.000	09:23
04 Std. Sol.	0.020	09:24
05 Room Air	0.000	09:25
06 Std. Sol.	0.020	09:25
07 Room Air	0.000	09:26

08 Sim Temp = 34.0°C

Simul Ser No = MP3064  
Std Sol No = 20070  
County = 08                            Oper No. = 666666

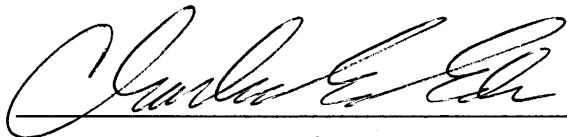

Operator Signature  
CHARLES EDER

Remarks: *Low AC*  
*0.020 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004184  
Location = TOXL                    8164.14.00 09/16  
05/17/2021                            09:28

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:28
02 Std. Sol.	0.296	09:29
03 Room Air	0.000	09:30
04 Std. Sol.	0.297	09:31
05 Room Air	0.000	09:31
06 Std. Sol.	0.298	09:32
07 Room Air	0.000	09:32

08 Sim Temp = 34.0°C

Simul Ser No = MP5317  
Std Sol No = 202012A  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*HIGH AC*  
*0.300 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-004184  
Location = TOXL                              8164.14.00 09/16  
05/17/2021    09:34

Test	AC	Time
01 Room Air	0.000	09:35
02 *Subject Test	INT*	09:36
03 Room Air	0.000	09:36

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 02/01/1992  
Sub Sex = Female                              Weight = 150  
Test = DUI                                      Cit = INTERFERENT  
Dr. Lic. = ND/DIS921456  
Lot No = 02621080A1  
Cyl No = 25  
Expiration Date = 03/05/2023  
County = 08                                      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *Interferent Check*  
*0.10AC + 0.05% ACETONE*

Form 106-18000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-004184  
Location = TOXL                              8164.14.00 09/16  
05/17/2021    09:37

Test	AC	Time
01 Diagnostic	OK	09:38
02 Room Air	0.000	09:39
03 *Subject Test	RFI*	09:39
04 Room Air	0.000	09:39

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 02/01/1992  
Sub Sex = Female                              Weight = 150  
Test = DUI                                      Cit = RFI CHECK  
Dr. Lic. = ND/DIS921456  
Lot No = 02621080A1  
Cyl No = 25  
Expiration Date = 03/05/2023  
County = 08                                      Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004184  
Location = TOXL      8164.14.00 09/16  
05/17/2021      09:44

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:44
02 Std. Gas	0.079	09:45
03 Room Air	0.000	09:45
04 Std. Gas	0.079	09:46
05 Room Air	0.000	09:46
06 Std. Gas	0.079	09:47
07 Room Air	0.000	09:47

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-004184  
Location = TOXL                                      8164.14.00 09/16  
05/17/2021    09:47

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:48
02 Std. Gas	0.078	09:48
03 Room Air	0.000	09:49
04 Std. Gas	0.079	09:49
05 Room Air	0.000	09:50
06 Std. Gas	0.079	09:50
07 Room Air	0.000	09:51

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08                                      Oper No. = 666666

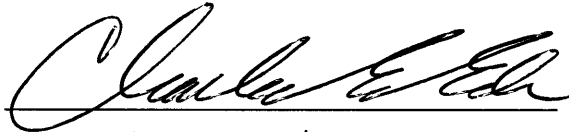

Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-004184  
Location = TOXL                                      8164.14.00 09/16  
05/17/2021    09:51

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:51
02 Std. Gas	0.079	09:52
03 Room Air	0.000	09:52
04 Std. Gas	0.079	09:53
05 Room Air	0.000	09:53
06 Std. Gas	0.079	09:53
07 Room Air	0.000	09:54

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08                                      Oper No. = 666666

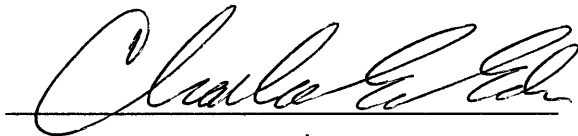

Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000