

**INTOXILYZER® 8000 INSPECTION**

Intoxilyzer® 8000 Serial Number: 80-005958 Location: TOXL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 222 psi Regulator: 250 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
  - a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.020 AC  
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
  - b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.300 AC  
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR3847 Lot #: FCS6 Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 02621080A1 Cyl #: 25 Exp. Date: 3.5.23

|                      |              |        |              |        |              |
|----------------------|--------------|--------|--------------|--------|--------------|
| Test 1               | <u>0.078</u> | Test 4 | <u>0.079</u> | Test 7 | <u>0.079</u> |
| Test 2               | <u>0.078</u> | Test 5 | <u>0.078</u> | Test 8 | <u>0.078</u> |
| Test 3               | <u>0.078</u> | Test 6 | <u>0.077</u> | Test 9 | <u>0.078</u> |
| Average <u>0.078</u> |              |        |              |        |              |

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED EXTERNAL BATTERY.

Instrument is acceptable to be used in the field.

Charles E. Ehr  
Breath Analyst Signature

5-18-21  
Date

Karl J. Diet  
Reviewed by

5-18-21  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005958  
Location = TOXL                 8164.14.00 09/16  
05/18/2021                        09:33

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%&\*()\_+?

Current Instrument Setup


Data Entry Mode:                Enabled  
Start Test Sequence:            DABACABA  
Display Prelim Rslt?            Yes  
Display Third Digit?            Yes  
Inhib Printer(Y/N)?            No  
Display Volume?                No  
Disable On Memfull?            Yes  
# of Print Copies?              1  
Select Std (D/W/I)?            Dry  
Standard Value?                0.080  
Standard Lot #?                 24119080A1  
Standard Cyl #?                20  
Standard Expiration?           11/05/2021  
Oper No?                        666666

Flow Cal. Date:                06/21/2013  
Slope                            716  
Intercept                       -760436

IR Calibration Date:           04/07/2015

|                    | 3um    | 9um    |
|--------------------|--------|--------|
| 0th Coef(*100):    | -17179 | -17694 |
| 1st Coef(*100):    | 259328 | 130890 |
| 2nd Coef(*100):    | 3473   | 1654   |
| H2O adj(mg/l*10k): | 425    | 422    |

\*\*\*\*\* Printer Test End \*\*\*\*\*

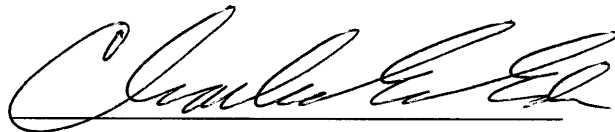

Operator Signature  
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005958  
Location = TOXL      8164.14.00 09/16  
05/18/2021      09:36

WET CAL CHECK

| Test         | AC    | Time  |
|--------------|-------|-------|
| 01 Room Air  | 0.000 | 09:37 |
| 02 Std. Sol. | 0.018 | 09:38 |
| 03 Room Air  | 0.000 | 09:38 |
| 04 Std. Sol. | 0.018 | 09:39 |
| 05 Room Air  | 0.000 | 09:39 |
| 06 Std. Sol. | 0.018 | 09:40 |
| 07 Room Air  | 0.000 | 09:41 |

08 Sim Temp = 34.0°C

Simul Ser No = MP3064  
Std Sol No = 20070  
County = 08      Oper No. = 666666

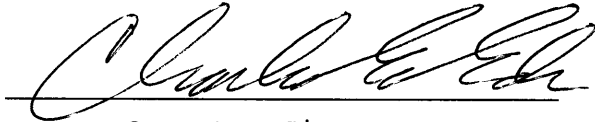

Operator Signature  
CHARLES EDER

Remarks:

Low AC  
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005958  
Location = TOXL      8164.14.00 09/16  
05/18/2021      09:46

WET CAL CHECK

| Test         | AC    | Time  |
|--------------|-------|-------|
| 01 Room Air  | 0.000 | 09:47 |
| 02 Std. Sol. | 0.293 | 09:47 |
| 03 Room Air  | 0.000 | 09:48 |
| 04 Std. Sol. | 0.293 | 09:49 |
| 05 Room Air  | 0.000 | 09:49 |
| 06 Std. Sol. | 0.294 | 09:50 |
| 07 Room Air  | 0.000 | 09:50 |

08 Sim Temp = 34.0°C

Simul Ser No = MP5317  
Std Sol No = 202012A  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:      HIGH AC  
                    0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005958  
Location = TOXL      8164.14.00 09/16  
05/18/2021      09:52

| Test             | AC    | Time  |
|------------------|-------|-------|
| 01 Room Air      | 0.000 | 09:53 |
| 02 *Subject Test | INT*  | 09:53 |
| 03 Room Air      | 0.000 | 09:54 |

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/08/1987  
Sub Sex = Male      Weight = 150  
Test = DUI      Cit = INTERFERENT  
Dr. Lic. = ND/DIS871456  
Lot No = 02621080A1  
Cyl No = 25  
Expiration Date = 03/05/2023  
County = 08      Oper No. = 666666

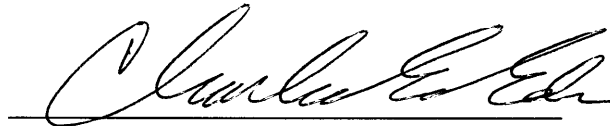

Operator Signature  
CHARLES EDER

Remarks: *Interferent Check*  
*0.10 AC + 0.05% ACETONE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005958  
Location = TOXL      8164.14.00 09/16  
05/18/2021      09:54

| Test             | AC    | Time  |
|------------------|-------|-------|
| 01 Diagnostic    | OK    | 09:55 |
| 02 Room Air      | 0.000 | 09:55 |
| 03 *Subject Test | RFI*  | 09:55 |
| 04 Room Air      | 0.000 | 09:56 |

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/08/1987  
Sub Sex = Male      Weight = 150  
Test = DUI      Cit = RFI CHECK  
Dr. Lic. = ND/DIS871456  
Lot No = 02621080A1  
Cyl No = 25  
Expiration Date = 03/05/2023  
County = 08      Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005958  
Location = TOXL      8164.14.00 09/16  
05/18/2021      09:56

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 09:57 |
| 02 Std. Gas | 0.078 | 09:57 |
| 03 Room Air | 0.000 | 09:58 |
| 04 Std. Gas | 0.078 | 09:58 |
| 05 Room Air | 0.000 | 09:58 |
| 06 Std. Gas | 0.078 | 09:59 |
| 07 Room Air | 0.000 | 09:59 |

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005958  
Location = TOXL      8164.14.00 09/16  
05/18/2021      10:00

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 10:00 |
| 02 Std. Gas | 0.079 | 10:01 |
| 03 Room Air | 0.000 | 10:01 |
| 04 Std. Gas | 0.078 | 10:01 |
| 05 Room Air | 0.000 | 10:02 |
| 06 Std. Gas | 0.077 | 10:02 |
| 07 Room Air | 0.000 | 10:03 |

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005958  
Location = TOXL      8164.14.00 09/16  
05/18/2021      10:03

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 10:04 |
| 02 Std. Gas | 0.079 | 10:04 |
| 03 Room Air | 0.000 | 10:04 |
| 04 Std. Gas | 0.078 | 10:05 |
| 05 Room Air | 0.000 | 10:05 |
| 06 Std. Gas | 0.078 | 10:06 |
| 07 Room Air | 0.000 | 10:06 |

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666

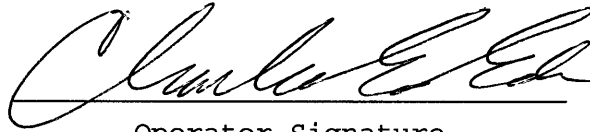

Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000