

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006500

Location: ToxL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 219 psi Regulator: 225 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
  - a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.030 AC  
Sim. Ser #: MP5289 Lot #: 201911E Exp. Date: 11.19.21
  - b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.400 AC  
Sim. Ser #: MP3062 Lot #: 202105E Exp. Date: 3.24.23

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR3847 Lot #: 7CS6 Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 02621080A1 Cyl #: 14 Exp. Date: 3.5.23

Test 1	<u>0.081</u>	Test 4	<u>0.082</u>	Test 7	<u>0.082</u>
Test 2	<u>0.081</u>	Test 5	<u>0.082</u>	Test 8	<u>0.082</u>
Test 3	<u>0.081</u>	Test 6	<u>0.082</u>	Test 9	<u>0.082</u>
Average	<u>CEE 0.082</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED EXTERNAL BATTERY, FLASH UPDATE OF CORE VERSION 8164.13 to 8164.14. THIS ADDS ABILITY TO READ NEWEST DRIVER'S LICENSE FORMAT.

Instrument is acceptable to be used in the field.

Breath Analyst Signature

Reviewed by

Charles E. Ehr  
Kali L. Hilt

Date

Date

5/24/2021  
5/24/21



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006500  
Location = TOXL      8164.14.00 09/16  
05/24/2021      15:28

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:28
02 Std. Sol.	0.030	15:29
03 Room Air	0.000	15:30
04 Std. Sol.	0.031	15:30
05 Room Air	0.000	15:31
06 Std. Sol.	0.031	15:32
07 Room Air	0.000	15:32


08 Sim Temp = 34.0°C

Simul Ser No = MP5289

Std Sol No = 201911E

County = 08

Oper No. = 666666

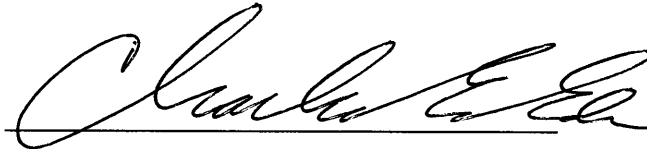

Operator Signature  
CHARLES EDER

Remarks:

Low AC  
0.030 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006500  
Location = TOXL      8164.14.00 09/16  
05/24/2021      15:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:35
02 Std. Sol.	0.406	15:35
03 Room Air	0.000	15:36
04 Std. Sol.	0.407	15:37
05 Room Air	0.000	15:37
06 Std. Sol.	0.407	15:38
07 Room Air	0.000	15:39

08 Sim Temp = 34.0°C

Simul Ser No = MP3062  
Std Sol No = 202103E  
County = 08      Oper No. = 666666

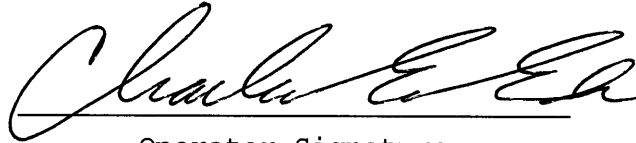

Operator Signature  
CHARLES EDER

Remarks:

HIGH AC  
0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006500  
Location = TOXL                    8164.14.00 09/16  
05/24/2021                            16:00

Test	AC	Time
01 Room Air	0.000	16:01
02 *Subject Test	INT*	16:02
03 Room Air	0.000	16:02

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 02/01/1992  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = INTERFERENT  
Dr. Lic. = ND/DIS921456  
Lot No = 02621080A1  
Cyl No = 14  
Expiration Date = 03/05/2023  
County = 08                            Oper No. = 666666

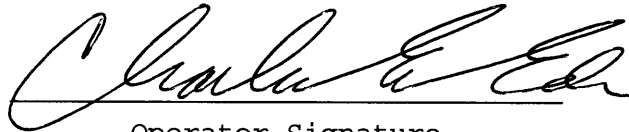

Operator Signature  
CHARLES EDER

Remarks:

*Interferent Check*  
*0.10 AC + 0.05% ACETONE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006500  
Location = TOXL                      8164.14.00 09/16  
05/24/2021                              16:05

Test	AC	Time
01 Diagnostic	OK	16:05
02 Room Air	0.000	16:06
03 *Subject Test	RFI*	16:06
04 Room Air	0.000	16:06

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 02/01/1992  
Sub Sex = Female                      Weight = 150  
Test = DUI                              Cit = RFI CHECK  
Dr. Lic. = ND/DIS921456  
Lot No = 02621080A1  
Cyl No = 14  
Expiration Date = 03/05/2023  
County = 08                              Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006500  
Location = TOXL      8164.14.00 09/16  
05/24/2021      16:07

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:07
02 Std. Gas	0.081	16:08
03 Room Air	0.000	16:08
04 Std. Gas	0.081	16:09
05 Room Air	0.000	16:09
06 Std. Gas	0.081	16:10
07 Room Air	0.000	16:10

Lot No = 02621080A1  
Cyl No = 14  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*CALIBRATION CHECK*  
*0.080 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006500  
Location = TOXL      8164.14.00 09/16  
05/24/2021      16:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:14
02 Std. Gas	0.082	16:14
03 Room Air	0.000	16:15
04 Std. Gas	0.082	16:15
05 Room Air	0.000	16:16
06 Std. Gas	0.082	16:16
07 Room Air	0.000	16:16

Lot No = 02621080A1  
Cyl No = 14  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

CALIBRATION CHECK  
0.080 AC

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006500  
Location = TOXL      8164.14.00 09/16  
05/24/2021      16:17

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:17
02 Std. Gas	0.082	16:18
03 Room Air	0.000	16:18
04 Std. Gas	0.082	16:19
05 Room Air	0.000	16:19
06 Std. Gas	0.082	16:19
07 Room Air	0.000	16:20

Lot No = 02621080A1  
Cyl No = 14  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666

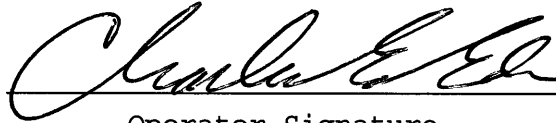

Operator Signature  
CHARLES EDER

Remarks:

CALIBRATION CHECK  
0.080 AC

Form 106-I8000