

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006504

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 204 psi Regulator: 225 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: JCS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 25 Exp. Date: 3.5.23

Test 1 <u>0.081</u>	Test 4 <u>0.081</u>	Test 7 <u>0.081</u>
Test 2 <u>0.091</u>	Test 5 <u>0.080</u>	Test 8 <u>0.080</u>
Test 3 <u>0.080</u>	Test 6 <u>0.081</u>	Test 9 <u>0.081</u>
Average <u>0.081</u>		

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED EXTERNAL BATTERY,

Instrument is acceptable to be used in the field.

Charles E. Ed
Breath Analyst Signature

5/29/21
Date

Kari L. Diet
Reviewed by

5/24/21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = TOXL 8164.14.00 09/16
05/24/2021 13:36

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNQPQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNQPQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 12
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 08/20/2015
Slope 681
Intercept -673151

IR Calibration Date: 05/31/2017

	3um	9um
0th Coef(*100):	-21488	-16160
1st Coef(*100):	265581	137324
2nd Coef(*100):	2507	1149
H2O adj(mg/l*10k):	519	348

***** Printer Test End *****

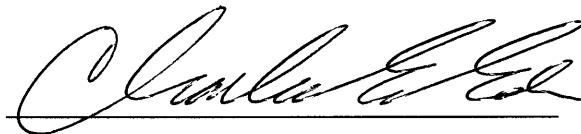

Operator Signature
CHARLES EDER

Remarks: *PRINT TEST*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = TOXL 8164.14.00 09/16
05/24/2021 13:39

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:39
02 Std. Sol.	0.019	13:40
03 Room Air	0.000	13:41
04 Std. Sol.	0.019	13:41
05 Room Air	0.000	13:42
06 Std. Sol.	0.019	13:43
07 Room Air	0.000	13:43

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

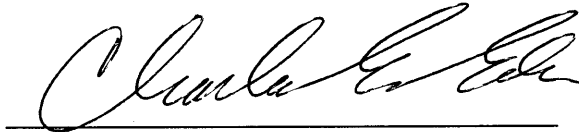

Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = TOXL 8164.14.00 09/16
05/24/2021 13:45

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:45
02 Std. Sol.	0.297	13:46
03 Room Air	0.000	13:47
04 Std. Sol.	0.299	13:47
05 Room Air	0.000	13:48
06 Std. Sol.	0.299	13:49
07 Room Air	0.000	13:49

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

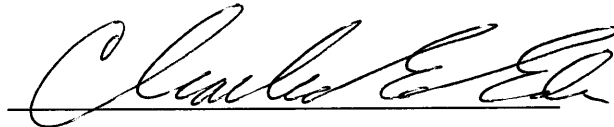

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = TOXL 8164.14.00 09/16
05/24/2021 13:50

Test	AC	Time
01 Room Air	0.000	13:51
02 *Subject Test	INT*	13:52
03 Room Air	0.000	13:52

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

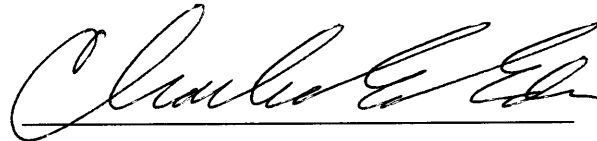

Operator Signature
CHARLES EDER

Remarks:

Interferent Clock
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = TOXL 8164.14.00 09/16
05/24/2021 13:53

Test	AC	Time
01 Diagnostic	OK	13:54
02 Room Air	0.000	13:54
03 *Subject Test	RFI*	13:54
04 Room Air	0.000	13:55

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

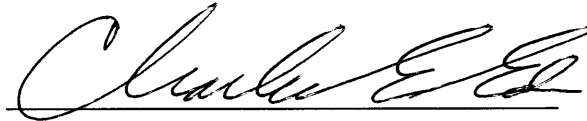

Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = TOXL 8164.14.00 09/16
05/24/2021 13:55

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:55
02 Std. Gas	0.081	13:56
03 Room Air	0.000	13:56
04 Std. Gas	0.081	13:57
05 Room Air	0.000	13:57
06 Std. Gas	0.080	13:58
07 Room Air	0.000	13:58

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = TOXL 8164.14.00 09/16
05/24/2021 13:58

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:59
02 Std. Gas	0.081	13:59
03 Room Air	0.000	14:00
04 Std. Gas	0.080	14:00
05 Room Air	0.000	14:01
06 Std. Gas	0.081	14:01
07 Room Air	0.000	14:02

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = TOXL 8164.14.00 09/16
05/24/2021 14:02

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:02
02 Std. Gas	0.081	14:03
03 Room Air	0.000	14:03
04 Std. Gas	0.080	14:04
05 Room Air	0.000	14:04
06 Std. Gas	0.081	14:04
07 Room Air	0.000	14:05

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

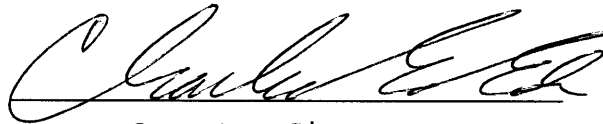

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080AC

Form 106-I8000