

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006491 Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 902 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 24119080A1 Cyl #: 31 Exp. Date: 11.5.21

Test 1	<u>0.082</u>	Test 4	<u>0.082</u>	Test 7	<u>0.082</u>
Test 2	<u>0.082</u>	Test 5	<u>0.082</u>	Test 8	<u>0.082</u>
Test 3	<u>0.082</u>	Test 6	<u>0.083</u>	Test 9	<u>0.083</u>
Average <u>0.082</u>					

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED SIMULATOR RETURN O-RING.

Instrument is acceptable to be used in the field.

Charles E. Ehr
Breath Analyst Signature

5/27/2021
Date

Kali L. Diet
Reviewed by

6/1/21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/27/2021 15:28

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^&* () _ + ?

abcdefghijklmnopqrstuvwxy1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^&* () _ + ?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 05620080A1
Standard Cyl #? 12
Standard Expiration? 04/05/2022
Oper No? 666666

Flow Cal. Date: 05/22/2018
Slope 639
Intercept -618311

IR Calibration Date: 05/23/2018

	3um	9um
0th Coef(*100):	-23641	-17066
1st Coef(*100):	264855	137703
2nd Coef(*100):	2663	1471
H2O adj(mg/l*10k):	556	451

***** Printer Test End *****

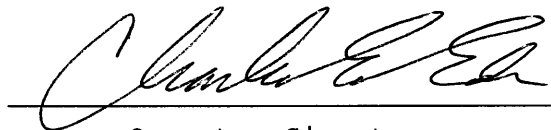

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/27/2021 15:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:34
02 Std. Sol.	0.019	15:35
03 Room Air	0.000	15:35
04 Std. Sol.	0.019	15:36
05 Room Air	0.000	15:37
06 Std. Sol.	0.020	15:37
07 Room Air	0.000	15:38

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

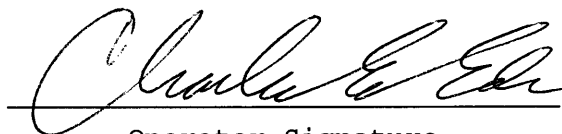

Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/27/2021 15:39

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:40
02 Std. Sol.	0.305	15:41
03 Room Air	0.000	15:41
04 Std. Sol.	0.304	15:42
05 Room Air	0.000	15:43
06 Std. Sol.	0.303	15:43
07 Room Air	0.000	15:44

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/27/2021 15:46

Test	AC	Time
01 Room Air	0.000	15:47
02 *Subject Test	INT*	15:47
03 Room Air	0.000	15:48

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 31
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/27/2021 15:49

Test	AC	Time
01 Diagnostic	OK	15:50
02 Room Air	0.000	15:50
03 *Subject Test	RFI*	15:51
04 Room Air	0.000	15:51

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 31
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/27/2021 15:51

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:52
02 Std. Gas	0.082	15:52
03 Room Air	0.000	15:53
04 Std. Gas	0.082	15:53
05 Room Air	0.000	15:54
06 Std. Gas	0.082	15:54
07 Room Air	0.000	15:55

Lot No = 24119080A1
Cyl No = 31
Exp Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/27/2021 15:55

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:56
02 Std. Gas	0.082	15:56
03 Room Air	0.000	15:57
04 Std. Gas	0.082	15:57
05 Room Air	0.000	15:58
06 Std. Gas	0.083	15:58
07 Room Air	0.000	15:59

Lot No = 24119080A1
Cyl No = 31
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

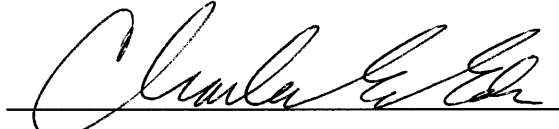
Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/27/2021 15:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:00
02 Std. Gas	0.082	16:00
03 Room Air	0.000	16:01
04 Std. Gas	0.082	16:01
05 Room Air	0.000	16:02
06 Std. Gas	0.083	16:02
07 Room Air	0.000	16:03

Lot No = 24119080A1
Cyl No = 31
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

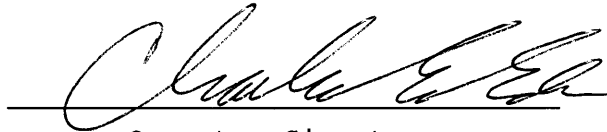

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000