

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006505

Location: TOXL

A. General Setup and Checks:

- 1. Diagnostic Tests Pass and Instrument in Ready Mode
- 2. Breath tube heated
- 3. Date, time and location code (Level 2,E). Re-set if necessary.
- 4. Print test (Level 1,P). Sign and attach test record.
- 5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 895 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

- 1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

- 2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS6 Exp. Date: NA
 Display reads "Interferent Detect"
- 3. RFI Check (CMS Mode) Display reads "RFI Detect"
- 4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 26 Exp. Date: 3.5.23
Test 1 0.081 Test 4 0.079 Test 7 0.080
Test 2 0.080 Test 5 0.080 Test 8 0.080
Test 3 0.080 Test 6 0.080 Test 9 0.080
Average 0.080

C. Remarks/Maintenance: ANNUAL INSPECTION, REMOVED
BROKEN PIECE OF MOUTHPIECE FROM BREATH HOSE END.

Instrument is acceptable to be used in the field.

Charles E. Eder
Breath Analyst Signature

6/2/21
Date

Kalvin D. Hieb
Reviewed by

6-7-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/02/2021 12:09

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 34
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 08/20/2015
Slope 671
Intercept -642269

IR Calibration Date: 08/20/2015

	3um	9um
0th Coef(*100):	-29025	-17051
1st Coef(*100):	252705	133345
2nd Coef(*100):	3840	1546
H2O adj(mg/l*10k):	817	461

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/02/2021 12:10

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:10
02 Std. Sol.	0.017	12:11
03 Room Air	0.000	12:11
04 Std. Sol.	0.018	12:12
05 Room Air	0.000	12:13
06 Std. Sol.	0.018	12:13
07 Room Air	0.000	12:14

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

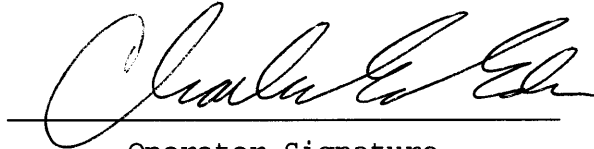

Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/02/2021 12:15

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:16
02 Std. Sol.	0.300	12:16
03 Room Air	0.000	12:17
04 Std. Sol.	0.302	12:18
05 Room Air	0.000	12:18
06 Std. Sol.	0.302	12:19
07 Room Air	0.000	12:20

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-18000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/02/2021 12:23

Test	AC	Time
01 Diagnostic	OK	12:23
02 Room Air	0.000	12:24
03 *Subject Test	RFI*	12:24
04 Room Air	0.000	12:25

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/02/2021 12:25

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:25
02 Std. Gas	0.081	12:26
03 Room Air	0.000	12:26
04 Std. Gas	0.080	12:27
05 Room Air	0.000	12:27
06 Std. Gas	0.080	12:27
07 Room Air	0.000	12:28


Lot No = 02621080A1

Cyl No = 26

Exp Date = 03/05/2023

County = 08

Oper No. = 666666

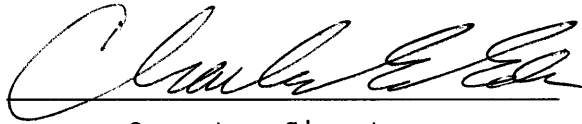

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/02/2021 12:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:29
02 Std. Gas	0.079	12:29
03 Room Air	0.000	12:30
04 Std. Gas	0.080	12:30
05 Room Air	0.000	12:31
06 Std. Gas	0.080	12:31
07 Room Air	0.000	12:32

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/02/2021 12:32

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:32
02 Std. Gas	0.080	12:33
03 Room Air	0.000	12:33
04 Std. Gas	0.080	12:34
05 Room Air	0.000	12:34
06 Std. Gas	0.080	12:34
07 Room Air	0.000	12:35

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

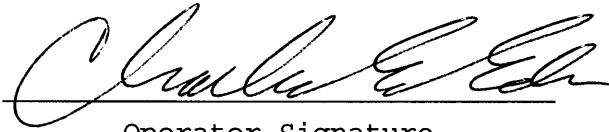

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000