

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-604189 Location: TOXL

- A. General Setup and Checks: 004198 KLH 6-10-21
1. Diagnostic Tests Pass and Instrument in Ready Mode
 2. Breath tube heated
 3. Date, time and location code (Level 2,E). Re-set if necessary.
 4. Print test (Level 1,P). Sign and attach test record.
 5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 877 psi Regulator: 900 psi

- B. Tests (Sign and attach test records):
- Configure simulator for the following tests (Level 1,S).
1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value \leq 0.03 AC: 0.015 AC
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
 - b. High AC (Level 1,C): Known Value \geq 0.25 AC: 0.400 AC
Sim. Ser #: MP3060 Lot #: 1910B Exp. Date: 10-20-21

- Configure dry gas standard for the following tests (Level 1,S).
2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7348 Lot #: 1C95 Exp. Date: NA
 Display reads "Interferent Detect"
 3. RFI Check (CMS Mode) Display reads "RFI Detect"
 4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 2419080A1 Cyl #: 033 Exp. Date: 11-9-21

Test 1 <u>0.081</u>	Test 4 <u>0.081</u>	Test 7 <u>0.080</u>
Test 2 <u>0.082</u>	Test 5 <u>0.080</u>	Test 8 <u>0.080</u>
Test 3 <u>0.081</u>	Test 6 <u>0.080</u>	Test 9 <u>0.080</u>
Average <u>0.080</u>		

C. Remarks/Maintenance: Annual inspection.
Replaced breath hose O-ring.

Instrument is acceptable to be used in the field.

Kelli L. Hib
Breath Analyst Signature 6-8-21
Date

Charles Egan
Reviewed by 6-10-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = TOXL 8164.14.00 09/16
06/08/2021 03:40

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 5
Standard Expiration? 02/05/2021
Oper No? 132598

Flow Cal. Date: 01/09/2012
Slope 637
Intercept -467208

	3um	9um
0th Coef(*100):	-19233	-23050
1st Coef(*100):	267031	132119
2nd Coef(*100):	2449	1142
H2O adj(mg/l*10k):	329	398

***** Printer Test End *****


Operator Signature
KALI HIEB

Remarks: *print test*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = TOXL 8164.14.00 09/16
06/08/2021 03:44

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	03:45
02 Std. Sol.	0.014	03:47
03 Room Air	0.000	03:48
04 Std. Sol.	0.014	03:49
05 Room Air	0.000	03:49
06 Std. Sol.	0.014	03:50
07 Room Air	0.000	03:50

08 Sim Temp = 34.0°C

Simul Ser No = MP5319
Std Sol No = 201911C
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: *wet cal check*
0.015 AC
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = TOXL 8164.14.00 09/16
06/08/2021 03:58

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	03:59
02 Std. Sol.	0.401	04:00
03 Room Air	0.000	04:00
04 Std. Sol.	0.402	04:01
05 Room Air	0.000	04:01
06 Std. Sol.	0.401	04:02
07 Room Air	0.000	04:03

08 Sim Temp = 33.9°C

Simul Ser No = MP3060
Std Sol No = 19108
County = 08 Oper No. = 132598

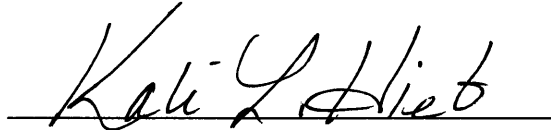

Operator Signature
KALI HIEB

Remarks: *wet cal check*
0.400 AC
Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = TOXL 8164.14.00 09/16
06/08/2021 04:07

Test	AC	Time
01 Room Air	0.000	04:08
02 *Subject Test	INT*	04:09
03 Room Air	0.000	04:09

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 24119080A1
Cyl No = 33
Expiration Date = 11/05/2021
County = 08 Oper No. = 132598

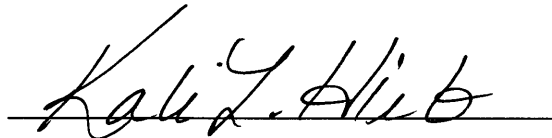
Operator Signature
KALI HIEB

Remarks: *Interferent check*
0.10AC + 0.059% Acetone
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = TOXL 8164.14.00 09/16
06/08/2021 04:10

Test	AC	Time
01 Diagnostic	OK	04:11
02 Room Air	0.000	04:12
03 *Subject Test	RFI*	04:12
04 Room Air	0.000	04:13

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 24119080A1
Cyl No = 33
Expiration Date = 11/05/2021
County = 08 Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

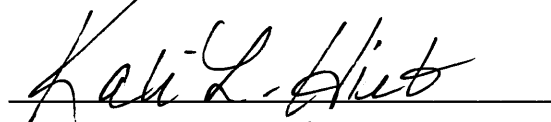
Operator Signature
KALI HIEB

Remarks: *RFI Check*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = TOXL 8164.14.00 09/16
06/08/2021 04:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	04:15
02 Std. Gas	0.081	04:15
03 Room Air	0.000	04:16
04 Std. Gas	0.082	04:16
05 Room Air	0.000	04:17
06 Std. Gas	0.081	04:17
07 Room Air	0.000	04:18

Lot No = 24119080A1
Cyl No = 33
Exp Date = 11/05/2021
County = 08 Oper No. = 132598

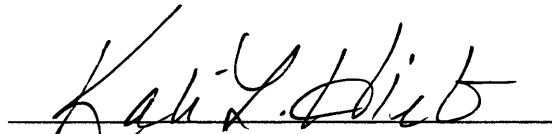
Operator Signature
KALI HIEB

Remarks: *Dry cal check*
O.D.B.O.A.C
Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = TOXL 8164.14.00 09/16
06/08/2021 04:21

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	04:21
02 Std. Gas	0.081	04:22
03 Room Air	0.000	04:22
04 Std. Gas	0.080	04:23
05 Room Air	0.000	04:23
06 Std. Gas	0.080	04:24
07 Room Air	0.000	04:24

Lot No = 24119080A1
Cyl No = 33
Exp Date = 11/05/2021
County = 08 Oper No. = 132598

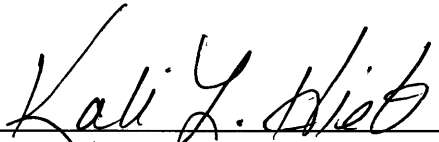

Operator Signature
KALI HIEB

Remarks: *Dry cal check*
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = TOXL 8164.14.00 09/16
06/08/2021 04:25

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	04:25
02 Std. Gas	0.080	04:26
03 Room Air	0.000	04:26
04 Std. Gas	0.080	04:27
05 Room Air	0.000	04:27
06 Std. Gas	0.080	04:27
07 Room Air	0.000	04:28

Lot No = 24119080A1
Cyl No = 33
Exp Date = 11/05/2021
County = 08 Oper No. = 132598

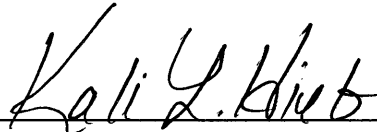

Operator Signature
KALI HIEB

Remarks:

*Dry cal check
0.080 AC*

Form 106-I8000