

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006506

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 197 psi Regulator: 200 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 11 Exp. Date: 3.5.23
Test 1 0.080 Test 4 0.080 Test 7 0.081
Test 2 0.080 Test 5 0.080 Test 8 0.080
Test 3 0.080 Test 6 0.080 Test 9 0.081
Average 0.080

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ed
Breath Analyst Signature

6/10/21
Date

Kali G. Dier
Reviewed by

6-14-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006506
Location = TOXL 8164.14.00 09/16
06/10/2021 10:17

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=-|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=-|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 02621080A1
Standard Cyl #? 11
Standard Expiration? 03/05/2023
Oper No? 666666

Flow Cal. Date: 08/20/2015
Slope 657
Intercept -627881

IR Calibration Date: 08/20/2015

	3um	9um
0th Coef(*100):	-22470	-18919
1st Coef(*100):	266505	136109
2nd Coef(*100):	3702	1644
H2O adj(mg/l*10k):	709	510

***** Printer Test End *****

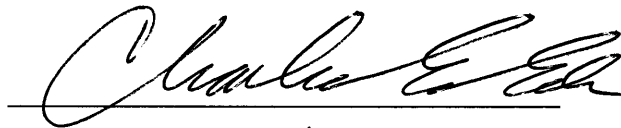

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006506
Location = TOXL 8164.14.00 09/16
06/10/2021 10:44

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:44
02 Std. Sol.	0.018	10:45
03 Room Air	0.000	10:45
04 Std. Sol.	0.018	10:46
05 Room Air	0.000	10:47
06 Std. Sol.	0.019	10:47
07 Room Air	0.000	10:48

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

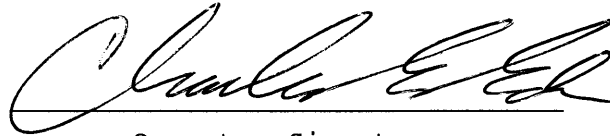

Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006506
Location = TOXL 8164.14.00 09/16
06/10/2021 10:49

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:50
02 Std. Sol.	0.297	10:51
03 Room Air	0.000	10:51
04 Std. Sol.	0.297	10:52
05 Room Air	0.000	10:52
06 Std. Sol.	0.298	10:53
07 Room Air	0.000	10:54

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

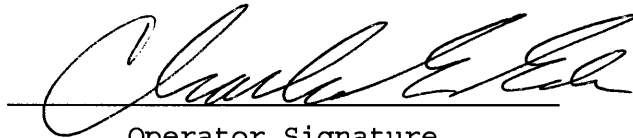

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006506
Location = TOXL 8164.14.00 09/16
06/10/2021 10:56

Test	AC	Time
01 Room Air	0.000	10:57
02 *Subject Test	INT*	10:57
03 Room Air	0.000	10:58

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 11
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

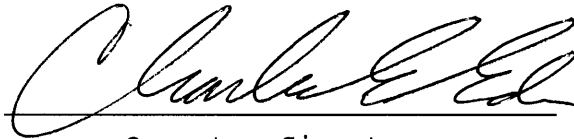

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006506
Location = TOXL 8164.14.00 09/16
06/10/2021 10:59

Test	AC	Time
01 Diagnostic	OK	11:00
02 Room Air	0.000	11:00
03 *Subject Test	RFI*	11:00
04 Room Air	0.000	11:01

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 11
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006506
Location = TOXL 8164.14.00 09/16
06/10/2021 11:01

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:01
02 Std. Gas	0.080	11:02
03 Room Air	0.000	11:02
04 Std. Gas	0.080	11:03
05 Room Air	0.000	11:03
06 Std. Gas	0.080	11:04
07 Room Air	0.000	11:04

Lot No = 02621080A1
Cyl No = 11
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

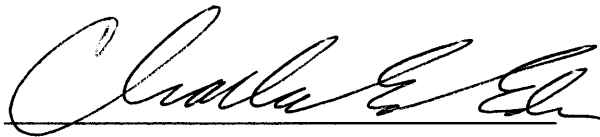

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006506
Location = TOXL 8164.14.00 09/16
06/10/2021 11:04

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:05
02 Std. Gas	0.080	11:05
03 Room Air	0.000	11:06
04 Std. Gas	0.080	11:06
05 Room Air	0.000	11:07
06 Std. Gas	0.080	11:07
07 Room Air	0.000	11:08

Lot No = 02621080A1
Cyl No = 11
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

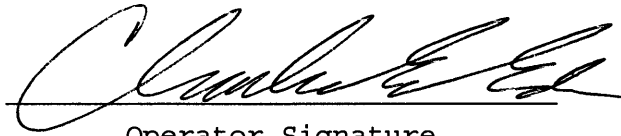

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006506
Location = TOXL 8164.14.00 09/16
06/10/2021 11:08

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:09
02 Std. Gas	0.081	11:09
03 Room Air	0.000	11:09
04 Std. Gas	0.080	11:10
05 Room Air	0.000	11:10
06 Std. Gas	0.081	11:11
07 Room Air	0.000	11:11

Lot No = 02621080A1
Cyl No = 11
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

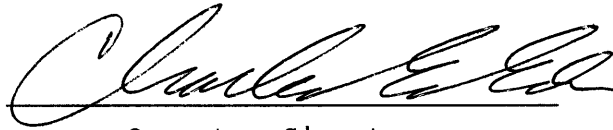

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080Ac
Form 106-I8000