

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-003072

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 174 psi Regulator: 200 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 05620080A1 Cyl #: 6 Exp. Date: 4.5.22

Test 1	<u>0.081</u>	Test 4	<u>0.082</u>	Test 7	<u>0.081</u>
Test 2	<u>0.081</u>	Test 5	<u>0.081</u>	Test 8	<u>0.082</u>
Test 3	<u>0.081</u>	Test 6	<u>0.081</u>	Test 9	<u>0.081</u>
Average	<u>0.081</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ed
Breath Analyst Signature

6/21/21
Date

Kali G. Hib
Reviewed by

6-22-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = TOXL 8164.14.00 09/16
06/21/2021 16:34

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 5
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 03/09/2011
Slope 682
Intercept -620512

IR Calibration Date: 03/09/2011

	3um	9um
0th Coef (*100):	-24766	-17499
1st Coef (*100):	264559	138630
2nd Coef (*100):	1876	1114
H2O adj (mg/l*10k):	497	331

***** Printer Test End *****

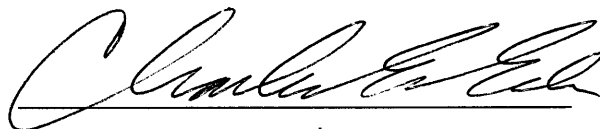

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = TOXL 8164.14.00 09/16
06/21/2021 16:35

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:36
02 Std. Sol.	0.019	16:36
03 Room Air	0.000	16:37
04 Std. Sol.	0.020	16:38
05 Room Air	0.000	16:38
06 Std. Sol.	0.019	16:39
07 Room Air	0.000	16:39

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

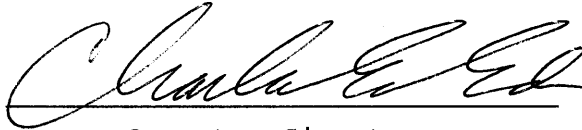

Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = TOXL 8164.14.00 09/16
06/21/2021 16:41

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:41
02 Std. Sol.	0.298	16:42
03 Room Air	0.000	16:42
04 Std. Sol.	0.298	16:43
05 Room Air	0.000	16:44
06 Std. Sol.	0.299	16:44
07 Room Air	0.000	16:45

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

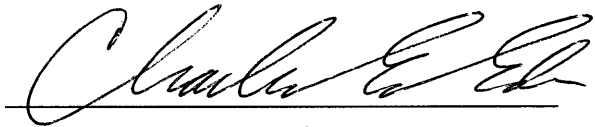

Operator Signature
CHARLES EDER

Remarks: HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = TOXL 8164.14.00 09/16
06/21/2021 16:46

Test	AC	Time
01 Room Air	0.000	16:46
02 *Subject Test	INT*	16:47
03 Room Air	0.000	16:47

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 05620080A1
Cyl No = 6
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

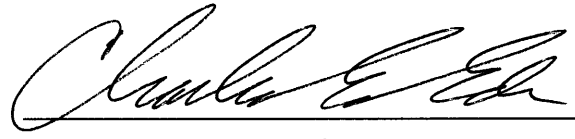

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = TOXL 8164.14.00 09/16
06/21/2021 16:48

Test	AC	Time
01 Diagnostic	OK	16:48
02 Room Air	0.000	16:49
03 *Subject Test	RFI*	16:49
04 Room Air	0.000	16:49

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 05620080A1
Cyl No = 6
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

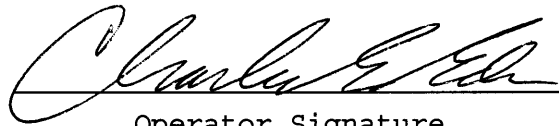

Operator Signature
CHARLES EDER

Remarks: RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = TOXL 8164.14.00 09/16
06/21/2021 16:50

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:50
02 Std. Gas	0.081	16:51
03 Room Air	0.000	16:51
04 Std. Gas	0.081	16:51
05 Room Air	0.000	16:52
06 Std. Gas	0.081	16:52
07 Room Air	0.000	16:53

Lot No = 05620080A1
Cyl No = 6
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

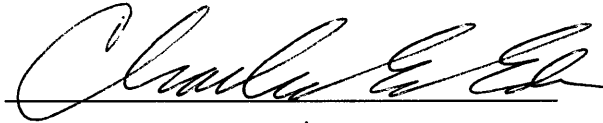

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = TOXL 8164.14.00 09/16
06/21/2021 16:53

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:53
02 Std. Gas	0.082	16:54
03 Room Air	0.000	16:54
04 Std. Gas	0.081	16:55
05 Room Air	0.000	16:55
06 Std. Gas	0.081	16:55
07 Room Air	0.000	16:56

Lot No = 05620080A1
Cyl No = 6
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

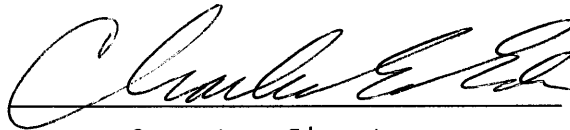

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = TOXL 8164.14.00 09/16
06/21/2021 16:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:57
02 Std. Gas	0.081	16:57
03 Room Air	0.000	16:58
04 Std. Gas	0.082	16:58
05 Room Air	0.000	16:59
06 Std. Gas	0.081	16:59
07 Room Air	0.000	16:59

Lot No = 05620080A1
Cyl No = 6
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

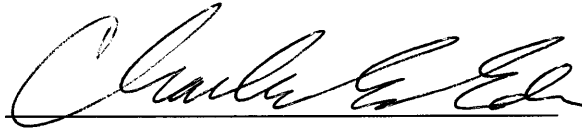

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000