

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-004199

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 215 psi Regulator: 225 psi

B. Tests (Sign and attach test records):

- Configure simulator for the following tests (Level 1,S).
1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: FCS6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 26 Exp. Date: 3.5.23

Test 1	<u>0.078</u>	Test 4	<u>0.079</u>	Test 7	<u>0.079</u>
Test 2	<u>0.079</u>	Test 5	<u>0.079</u>	Test 8	<u>0.079</u>
Test 3	<u>0.079</u>	Test 6	<u>0.079</u>	Test 9	<u>0.079</u>
Average <u>0.079</u>					

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ed
Breath Analyst Signature

6/21/21
Date

Kelli G. Hilt
Reviewed by

6-21-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/21/2021 12:19

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 5
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 06/17/2019
Slope 593
Intercept -481610

IR Calibration Date: 06/17/2019

	3um	9um
0th Coef (*100):	-17512	-19237
1st Coef (*100):	277207	136841
2nd Coef (*100):	1620	1027
H2O adj (mg/l*10k):	211	375

***** Printer Test End *****

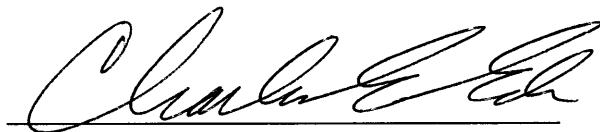

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/21/2021 12:21

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:22
02 Std. Sol.	0.021	12:22
03 Room Air	0.000	12:23
04 Std. Sol.	0.020	12:24
05 Room Air	0.000	12:24
06 Std. Sol.	0.021	12:25
07 Room Air	0.000	12:25

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

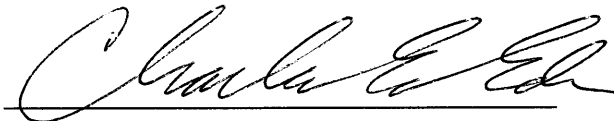

Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/21/2021 12:26

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:27
02 Std. Sol.	0.297	12:27
03 Room Air	0.000	12:28
04 Std. Sol.	0.299	12:29
05 Room Air	0.000	12:29
06 Std. Sol.	0.299	12:30
07 Room Air	0.000	12:31

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

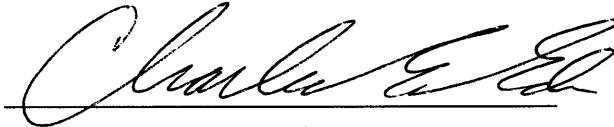

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/21/2021 12:37

Test	AC	Time
01 Room Air	0.000	12:38
02 *Subject Test	INT*	12:38
03 Room Air	0.000	12:39

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/21/2021 12:39

Test	AC	Time
01 Diagnostic	OK	12:40
02 Room Air	0.000	12:41
03 *Subject Test	RFI*	12:41
04 Room Air	0.000	12:41

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

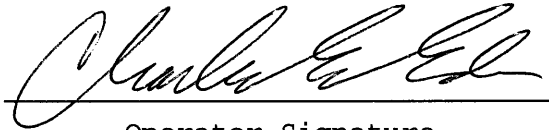

Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/21/2021 12:45

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:45
02 Std. Gas	0.078	12:46
03 Room Air	0.000	12:46
04 Std. Gas	0.079	12:47
05 Room Air	0.000	12:47
06 Std. Gas	0.079	12:48
07 Room Air	0.000	12:48

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

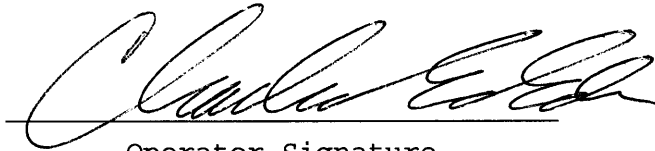

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/21/2021 12:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:49
02 Std. Gas	0.079	12:49
03 Room Air	0.000	12:50
04 Std. Gas	0.079	12:50
05 Room Air	0.000	12:50
06 Std. Gas	0.079	12:51
07 Room Air	0.000	12:51

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

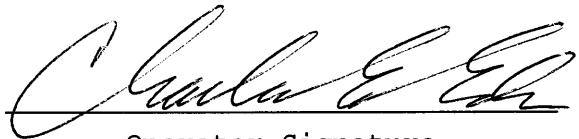

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/21/2021 12:52

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:52
02 Std. Gas	0.079	12:53
03 Room Air	0.000	12:53
04 Std. Gas	0.079	12:53
05 Room Air	0.000	12:54
06 Std. Gas	0.079	12:54
07 Room Air	0.000	12:55

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000