

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-003065 Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 94 psi Regulator: 100 psi

B. Tests (Sign and attach test records):

- Configure simulator for the following tests (Level 1,S).
1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2-13-22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12-8-22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 26 Exp. Date: 3.5.23

Test 1	<u>0.079</u>	Test 4	<u>0.078</u>	Test 7	<u>0.079</u>
Test 2	<u>0.079</u>	Test 5	<u>0.078</u>	Test 8	<u>0.079</u>
Test 3	<u>0.079</u>	Test 6	<u>0.079</u>	Test 9	<u>0.078</u>
Average	<u>0.079</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Hest
Breath Analyst Signature

6/22/21
Date

Kali G. Hest
Reviewed by

6-22-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 15:09

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 5
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 05/19/2017
Slope 612
Intercept 21223

IR Calibration Date: 08/23/2016

	3um	9um
0th Coef(*100):	-14934	-12309
1st Coef(*100):	289519	141483
2nd Coef(*100):	1834	736
H2O adj(mg/l*10k):	268	136

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 15:10

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:11
02 Std. Sol.	0.020	15:12
03 Room Air	0.000	15:12
04 Std. Sol.	0.020	15:13
05 Room Air	0.000	15:13
06 Std. Sol.	0.020	15:14
07 Room Air	0.000	15:15

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 15:26

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:26
02 Std. Sol.	0.296	15:27
03 Room Air	0.000	15:28
04 Std. Sol.	0.299	15:28
05 Room Air	0.000	15:29
06 Std. Sol.	0.298	15:30
07 Room Air	0.000	15:30

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

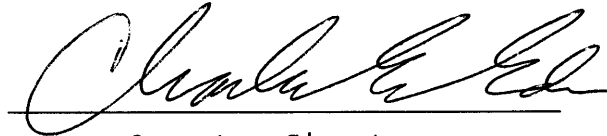

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 15:33

Test	AC	Time
01 Room Air	0.000	15:33
02 *Subject Test	INT*	15:34
03 Room Air	0.000	15:34

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 15:35

Test	AC	Time
01 Diagnostic	OK	15:36
02 Room Air	0.000	15:37
03 *Subject Test	RFI*	15:37
04 Room Air	0.000	15:37

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 15:38

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:38
02 Std. Gas	0.079	15:38
03 Room Air	0.000	15:39
04 Std. Gas	0.079	15:39
05 Room Air	0.000	15:40
06 Std. Gas	0.079	15:40
07 Room Air	0.000	15:41

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

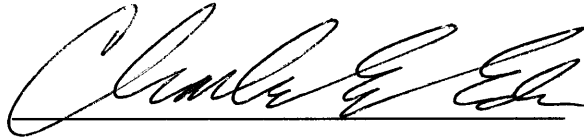

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 15:41

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:42
02 Std. Gas	0.078	15:42
03 Room Air	0.000	15:43
04 Std. Gas	0.078	15:43
05 Room Air	0.000	15:44
06 Std. Gas	0.079	15:44
07 Room Air	0.000	15:45

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

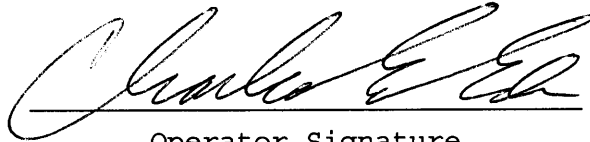

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 15:45

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:45
02 Std. Gas	0.079	15:46
03 Room Air	0.000	15:46
04 Std. Gas	0.079	15:47
05 Room Air	0.000	15:47
06 Std. Gas	0.078	15:48
07 Room Air	0.000	15:48


Lot No = 02621080A1

Cyl No = 26

Exp Date = 03/05/2023

County = 08

Oper No. = 666666

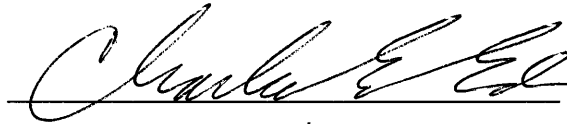

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000