

- 5. Temperature Monitor (Level 3,D,T): C: 47.0 A: 49.5 I: 0.0
B: 45.1 V: 0.0
- 6. Tank Monitor (Level 3,D,G): P (display): 150 psi P (gauge): 175 psi
- 7. General Setup (Level 3,S,G)
- 8. Configure Start Test (Level 3,S,T)
- 9. Network (Level 3,S,N)

E. TESTS (attach all test records):

Configure wet bath simulator standards before running tests (Level 1,S):

- 1. Zero AC (Level 1,C):
Sim ser #: MP5320 Lot #: MILLIQ H2O Exp date: NA
Known value: 0.000 AC
Results: 0.000 AC 0.000 AC 0.000 AC
- 2. Low AC (Level 1,C):
Sim ser #: MP5289 Lot #: 201911E Exp date: 11.19.21
Known value: 0.030 AC
Results: 0.030 AC 0.030 AC 0.030 AC
- 3. High AC (Level 1,C):
Sim ser #: MP3061 Lot #: 20101 Exp date: 2.13.22
Known value: 0.500 AC
Results: 0.494 AC 0.495 AC 0.494 AC

Configure dry gas standard before running tests (Level 1,S):

- 4. Ethanol + 0.05% Acetone (Level 1,B):
Sim ser #: DR5114 Lot #: IC56 Exp date: NA
Known value: 0.10 AC + 0.05% ACETONE
 Display reads "Interferent Detect"
- 5. Acetone (Level 1,B):
Sim ser #: DR5188 Lot #: ACE1 Exp date: NA
Known value: 0.05% ACETONE
 Display reads "Interferent Detect"
- 6. Methanol (Level 1,B):
Sim ser #: DR5186 Lot #: MET3 Exp date: NA
Known value: 0.10% METHANOL
 Display reads "Interferent Detect"
- 7. Isopropanol (Level 1,B):
Sim ser #: DR5189 Lot #: IPA2 Exp date: NA
Known value: 0.10% ISOPROPANOL
 Display reads "Interferent Detect"

- 8. Ambient Fail (Level 1,B): Display and test record read correct.
- 9. Invalid Sample (Level 1,B): Display and test record read correct.
- 10. Sequence Aborted (Level 1,B): Display and test record read correct.
- 11. ABA (Level 1,B): Test record reads correct.
- 12. Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- 13. RFI Detected (B,C, or CMS mode): Display and test record read correct.
- 14. Tank Pressure Below Minimum (CMS mode): Display reads correct.
- 15. Deficient Samples (CMS mode): Display and test record read correct.
- 16. Improper Sample (CMS mode): Display and test record read correct.
- 17. Difference Too Great (CMS mode): Display and test record read correct.
- 18. CMS (CMS mode): Test record reads correct.
- 19. Stability Test (Level 3,T,S):

Ave: 0.0790 Std Dev: 0.0006 Rel Std Dev: 0.72%

Maintenance/Repairs/Notes: INITIAL INSPECTION DUE TO OPENING
UP INSTRUMENT TO REPLACE REAL TIME CLOCK BATTERY.
REPLACED SIMULATOR RETURN O-RING.

Instrument is acceptable to be used in the field.

Charles E. Ed
Field Inspector's Signature

6/22/21
Date

Kali L. Hieb
Reviewed by

6-22-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 12:30

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

24 characters per line
abcdefghijklmnopqrstuwx
ABCDEFGHIJKLMNQRSTUWX

32 characters per line
abcdefghijklmnopqrstuwx123456
ABCDEFGHIJKLMNQRSTUWXYZ123456

42 characters per line
abcdefghijklmnopqrstuwx1234567890abcdef
ABCDEFGHIJKLMNQRSTUWXYZ1234567890ABCDEF


Current Instrument Setup
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On MemFull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 5
Standard Expiration? 02/05/2021
Oper No? 666666

Flow Cal. Date: 05/19/2017
Slope: 612
Intercept: 21223

IR Calibration Date: 08/23/2016
3um 9um

0th Coef(*100): -14934 -12309
1st Coef(*100): 289519 141483
2nd Coef(*100): 1834 736
H2O adj(mg/l)*10K: 268 136

***** Test End *****



Operator Signature
CHARLES EDER

Remarks: **INTERNAL
PRINT TEST**

Form 106-18000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 12:35

Test	AC	Time
01 Room Air	0.000	12:36
02 *Subject Test	REF*	12:37
03 Room Air	0.000	12:37

*Subject Test Refused

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = R KEY REFUSAL
Dr. Lic. = ND/TES989643
Lot No = 34418080A2
Cyl No = 5
Expiration Date = 02/05/2021
County = 08 Oper No. = 666666

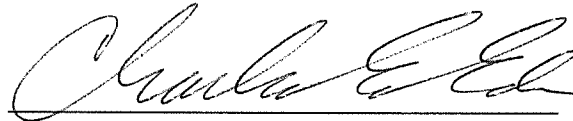

Operator Signature
CHARLES EDER

Remarks: "R" KEY REFUSAL

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 12:38

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666

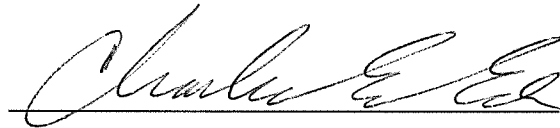

Operator Signature
CHARLES EDER

Remarks:

DIAGNOSTIC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 12:45

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:45
02 Std. Sol.	0.000	12:46
03 Room Air	0.000	12:46
04 Std. Sol.	0.000	12:47
05 Room Air	0.000	12:48
06 Std. Sol.	0.000	12:48
07 Room Air	0.000	12:49

08 Sim Temp = 34.0°C

Simul Ser No = MP5320
Std Sol No = MILLIQ H2O
County = 08 Oper No. = 666666

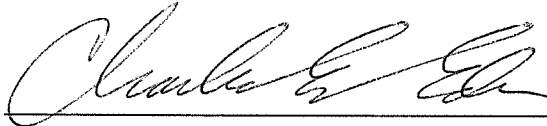

Operator Signature
CHARLES EDER

Remarks: ZERO AC
 0.000 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 12:51

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:51
02 Std. Sol.	0.030	12:52
03 Room Air	0.000	12:53
04 Std. Sol.	0.030	12:53
05 Room Air	0.000	12:54
06 Std. Sol.	0.030	12:55
07 Room Air	0.000	12:55

08 Sim Temp = 34.0°C

Simul Ser No = MP5289

Std Sol No = 201911E

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC
0.030 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:02

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:02
02 Std. Sol.	0.494	13:03
03 Room Air	0.000	13:04
04 Std. Sol.	0.495	13:05
05 Room Air	0.000	13:05
06 Std. Sol.	0.494	13:06
07 Room Air	0.000	13:06

08 Sim Temp = 34.0°C

Simul Ser No = MP3061
Std Sol No = 20101
County = 08 Oper No. = 666666

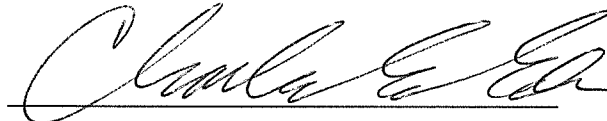

Operator Signature
CHARLES EDER

Remarks: HIGH AC
 0.500 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:08

Test	AC	Time
01 Room Air	0.000	13:09
02 *Subject Test	INT*	13:09
03 Room Air	0.000	13:10

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

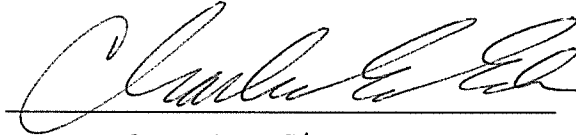

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10 AC + 0.05% ACETONE

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:10

Test	AC	Time
01 Room Air	0.000	13:11
02 *Subject Test	INT*	13:11
03 Room Air	0.000	13:12

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

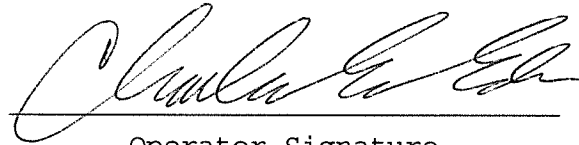

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.05% ACETONE

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:13

Test	AC	Time
01 Room Air	0.000	13:14
02 *Subject Test	INT*	13:14
03 Room Air	0.000	13:15

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10% METHANOL

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:15

Test	AC	Time
01 Room Air	0.000	13:16
02 *Subject Test	INT*	13:16
03 Room Air	0.000	13:17

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10% ISOPROPANOL
Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:21

Test	AC	Time
01 Room Air	AMB*	13:21
02 Room Air	0.000	13:22

*Invalid Test
Check Ambient Conditions

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = AMBIENT FAIL
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

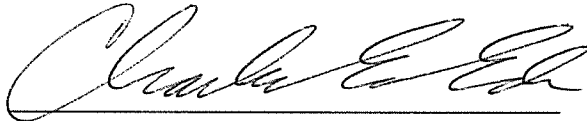

Operator Signature
CHARLES EDER

Remarks: *AMBIENT
 FAIL*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:22

Test	AC	Time
01 Room Air	0.000	13:23
02 Invalid Sample	X.XXX	13:24
03 Room Air	0.000	13:24

*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INVALID SAMPLE
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

INVALID
SAMPLE

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:25

Test	AC	Time
01 Room Air	0.000	13:26
02 *Subject Test	ABT*	13:26
03 Room Air	0.000	13:26

*Sequence Aborted

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = SEQUENCE ABORT
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: SEQUENCE
 ABORTED

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:29

Test	AC	Time
01 Room Air	0.000	13:30
02 Subject Test 1	0.189	13:30
03 Room Air	0.000	13:31
04 Reported AC	0.189	13:30

No RFI Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = ABA MODE TEST
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

*ABA MODE
TEST*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:32

Test	AC	Time
01 Diagnostic	OK	13:33
02 Room Air	0.000	13:33
03 Subject Test 1	0.187	13:33
04 Room Air	0.000	13:36
05 Std. Gas	0.086*	13:37
06 Room Air	0.000	13:37

*Cal Check Out of Tolerance

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = CAL CHK OUT TOL
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
OUT OF TOLERANCE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:39

Test	AC	Time
01 Diagnostic	OK	13:40
02 Room Air	0.000	13:40
03 *Subject Test	RFI*	13:40
04 Room Air	0.000	13:41

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:42

Test	AC	Time
01 Diagnostic	OK	13:43
02 Room Air	0.000	13:43
03 *Subject Test	0.000*	13:46
04 Room Air	0.000	13:48
05 Std. Gas	0.079	13:50
06 Room Air	0.000	13:51
07 *Subject Test	0.000*	13:54
08 Room Air	0.000	13:55


No RFI Detected

*Deficient Sample - Value Printed was
Highest Obtained

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = DEFICIENT SAMPL
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.

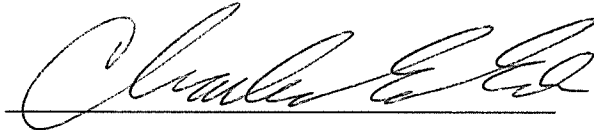

Operator Signature
CHARLES EDER

Remarks: DEFICIENT
SAMPLES

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 13:55

Test	AC	Time
01 Diagnostic	OK	13:56
02 Room Air	0.000	13:56
03 Reference	IPS*	13:56
04 Room Air	0.000	13:57

*Improper Sample

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = IMPROPER SAMPLE
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

*IMPROPER
SAMPLE*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 14:08

Test	AC	Time
01 Diagnostic	OK	14:08
02 Room Air	0.000	14:09
03 Subject Test 1	0.046*	14:09
04 Room Air	0.000	14:11
05 Std. Gas	0.079	14:13
06 Room Air	0.000	14:14
07 Subject Test 2	0.184*	14:15
08 Room Air	0.000	14:16

*Difference Too Great

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = DIFF TOO GREAT
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

DIFFERENCE
TOO GREAT

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 14:35

Test	AC	Time
01 Diagnostic	OK	14:36
02 Room Air	0.000	14:36
03 Subject Test 1	0.000	14:36
04 Room Air	0.000	14:38
05 Std. Gas	0.078	14:40
06 Room Air	0.000	14:41
07 Subject Test 2	0.000	14:41
08 Room Air	0.000	14:42
09 Reported AC	0.000	14:36

Difference OK
No RFI Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = CMS MODE TEST
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 5
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

CMS MODE
TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/22/2021 14:43

Test	AC	Time
01 Room Air	0.000	14:44
02 Std. Gas	0.079	14:44
03 Room Air	0.000	14:45
04 Std. Gas	0.078	14:45
05 Room Air	0.000	14:46
06 Std. Gas	0.078	14:46
07 Room Air	0.000	14:47
08 Std. Gas	0.079	14:47
09 Room Air	0.000	14:47
10 Std. Gas	0.078	14:48
11 Room Air	0.000	14:48
12 Std. Gas	0.079	14:49
13 Room Air	0.000	14:49
14 Std. Gas	0.079	14:49
15 Room Air	0.000	14:50
16 Std. Gas	0.079	14:50
17 Room Air	0.000	14:51
18 Std. Gas	0.079	14:51
19 Room Air	0.000	14:52
20 Std. Gas	0.079	14:52
21 Room Air	0.000	14:53
22 Std. Gas	0.079	14:53
23 Room Air	0.000	14:54
24 Std. Gas	0.079	14:54
25 Room Air	0.000	14:54
26 Std. Gas	0.079	14:55
27 Room Air	0.000	14:55
28 Std. Gas	0.080	14:56
29 Room Air	0.000	14:56
30 Std. Gas	0.080	14:57
31 Room Air	0.000	14:57
32 Std. Gas	0.079	14:57
33 Room Air	0.000	14:58
34 Std. Gas	0.079	14:58
35 Room Air	0.000	14:59
36 Std. Gas	0.079	14:59
37 Room Air	0.000	15:00
38 Std. Gas	0.080	15:00
39 Room Air	0.000	15:01
40 Std. Gas	0.079	15:01
41 Room Air	0.000	15:01
42 Cal Check Stats:		
43 Average	0.0790	
44 Std Dev	0.0006	
45 Rel Std Dev	0.72%	



Operator Signature
CHARLES EDER

Remarks: 0.080 AC

STABILITY TEST

Form 106-I8000

LOT: 29119080A1

CYL: 5

Exp: 11/5/2021