

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006492

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 977 psi Regulator: 975 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202001B Exp. Date: 1.28.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: IC56 Exp. Date: NA

Display reads "Interferent Detect"

3. RFI Check (CMS Mode) Display reads "RFI Detect"

4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC

Gas Cyl Lot #: 05620080A1 Cyl #: 6 Exp. Date: 4.5.22

Test 1 0.080 Test 4 0.080 Test 7 0.080

Test 2 0.080 Test 5 0.081 Test 8 0.080

Test 3 0.080 Test 6 0.080 Test 9 0.080

Average 0.080

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Breath Analyst Signature

Reviewed by

Date

Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006492
Location = TOXL 8164.14.00 09/16
06/28/2021 10:17

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 11
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 08/18/2015
Slope 669
Intercept -631515

IR Calibration Date: 08/18/2015

	3um	9um
0th Coef(*100):	-41685	-23145
1st Coef(*100):	269226	142194
2nd Coef(*100):	2671	1239
H2O adj(mg/l*10k):	872	437

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks: PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006492
Location = TOXL 8164.14.00 09/16
06/28/2021 10:20

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:21
02 Std. Sol.	0.018	10:21
03 Room Air	0.000	10:22
04 Std. Sol.	0.018	10:23
05 Room Air	0.000	10:23
06 Std. Sol.	0.018	10:24
07 Room Air	0.000	10:24

08 Sim Temp = 34.0°C

Simul Ser No = MP3064

Std Sol No = 20070

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006492
Location = TOXL 8164.14.00 09/16
06/28/2021 10:27

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:27
02 Std. Sol.	0.295	10:28
03 Room Air	0.000	10:29
04 Std. Sol.	0.296	10:29
05 Room Air	0.000	10:30
06 Std. Sol.	0.296	10:31
07 Room Air	0.000	10:31


08 Sim Temp = 34.0°C

Simul Ser No = MP5317

Std Sol No = 202001B

County = 08

Oper No. = 666666

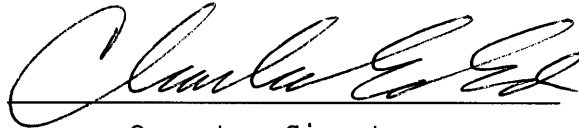

Operator Signature

CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006492
Location = TOXL 8164.14.00 09/16
06/28/2021 10:33

Test	AC	Time
01 Room Air	0.000	10:34
02 *Subject Test	INT*	10:34
03 Room Air	0.000	10:35

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 05620080A1
Cyl No = 6
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

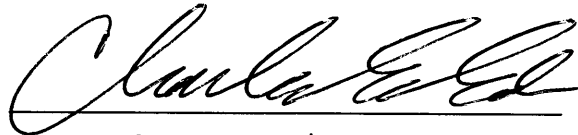

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006492
Location = TOXL 8164.14.00 09/16
06/28/2021 10:36

Test	AC	Time
01 Diagnostic	OK	10:37
02 Room Air	0.000	10:38
03 *Subject Test	RFI*	10:38
04 Room Air	0.000	10:38

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 05620080A1
Cyl No = 6
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

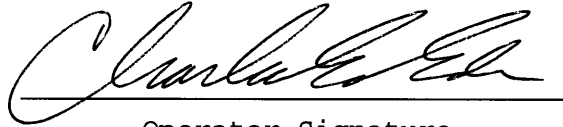

Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006492
Location = TOXL 8164.14.00 09/16
06/28/2021 10:39

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:39
02 Std. Gas	0.080	10:39
03 Room Air	0.000	10:40
04 Std. Gas	0.080	10:40
05 Room Air	0.000	10:41
06 Std. Gas	0.080	10:41
07 Room Air	0.000	10:42

Lot No = 05620080A1
Cyl No = 6
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

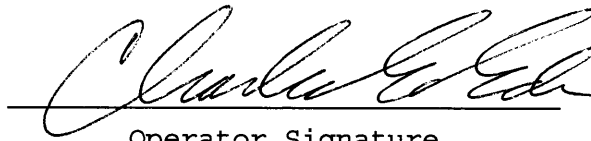

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006492
Location = TOXL 8164.14.00 09/16
06/28/2021 10:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:43
02 Std. Gas	0.080	10:43
03 Room Air	0.000	10:44
04 Std. Gas	0.081	10:44
05 Room Air	0.000	10:45
06 Std. Gas	0.080	10:45
07 Room Air	0.000	10:45

Lot No = 05620080A1
Cyl No = 6
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

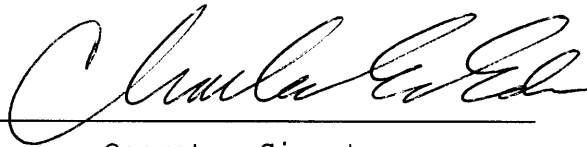

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006492
Location = TOXL 8164.14.00 09/16
06/28/2021 10:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:46
02 Std. Gas	0.080	10:47
03 Room Air	0.000	10:47
04 Std. Gas	0.080	10:48
05 Room Air	0.000	10:48
06 Std. Gas	0.080	10:49
07 Room Air	0.000	10:49

Lot No = 05620080A1
Cyl No = 6
Exp Date = 04/05/2022
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000