



ETHANOL GAS STANDARD CYLINDER REPORT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59282 (08/2018)

Chemical Test Operator Name (Print) <i>Rathryn Allen</i>		
Location <i>Cass County Jail-Booking</i>	Intoxilyzer® Serial Number <i>80-005944</i>	
Gas Lot Number <i>02621080A1</i>	Gas Cylinder Number <i>27</i>	Gas Expiration Date <i>3/5/2023</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
 Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 A. 0.*083* AC
 B. 0.*083* AC
 C. 0.*082* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
 B. ACA Test Record.

Chemical Test Operator Signature <i>Rathryn Allen #3671</i>	Date <i>1-25-22</i>
Reviewed By (Crime Laboratory Use Only) <i>Charles E. Edr</i>	Date <i>1/27/22</i>

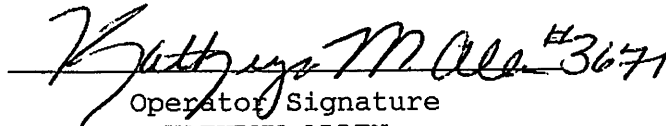
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005944
Location = CASS 8164.14.00 09/16
01/25/2022 15:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:16
02 Std. Gas	0.083	15:17
03 Room Air	0.000	15:17
04 Std. Gas	0.083	15:17
05 Room Air	0.000	15:18
06 Std. Gas	0.082	15:18
07 Room Air	0.000	15:19

Lot No = 02621080A1
Cyl No = 27
Exp Date = 03/05/2023
County = 09 Oper No. = 090801


Operator Signature
KATHRYN ALLEN

Remarks:

Form 106-I8000

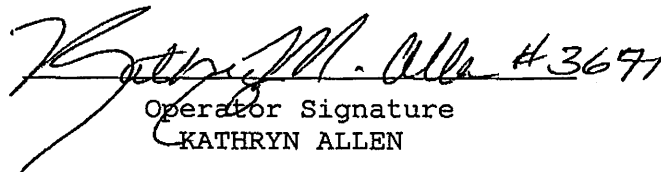
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005944
Location = CASS 8164.14.00 09/16
01/25/2022 15:20

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 090801

 #3671
Operator Signature
KATHRYN ALLEN

Remarks:

Form 106-I8000