



# INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM

SFN 59281 (06/2018)

Serial Number <b>80-005360</b>	Instrument Location <b>GFPD</b>
Reason for Install/Repair	
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

### Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): none
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>Jon Lampi</i>	Date <i>07-20-22</i>
---	-------------------------

### Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By <i>Janelle Portschiller</i>	Certified Date <i>08/01/2022</i>
--	-------------------------------------

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005360  
Location = GFPD                8164.14.00 09/16  
07/20/2022                      09:42

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup

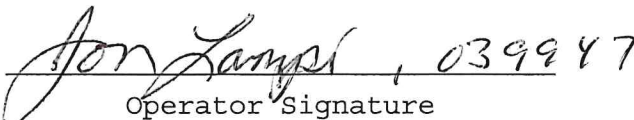
Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?         1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            02621080A1  
Standard Cyl #?            35  
Standard Expiration?       03/05/2023  
Oper No?                    039947

Flow Cal. Date:            06/16/2021  
Slope                        517  
Intercept                  187172

IR Calibration Date:       06/16/2021  
                                  3um                    9um

-----  
0th Coef(\*100):            -7908                    -18879  
1st Coef(\*100):            270905                  148636  
2nd Coef(\*100):            959                      696  
H2O adj(mg/l\*10k):        168                      275

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
Operator Signature  
JONATHAN LAMPI

Remarks:

Form 106-I8000  
Annual Inspection  
Install print test


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005360  
Location = GFPD      8164.14.00 09/16  
07/20/2022      09:43

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:43
02 Std. Gas	0.079	09:44
03 Room Air	0.000	09:44
04 Std. Gas	0.078	09:45
05 Room Air	0.000	09:45
06 Std. Gas	0.079	09:45
07 Room Air	0.000	09:46

Lot No = 02621080A1  
Cyl No = 35  
Exp Date = 03/05/2023  
County = 18      Oper No. = 039947

  
Operator Signature  
JONATHAN LAMPI

Remarks:

Form 106-I8000

Annual Inspection  
Install ACH TEST

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005360  
Location = GFPD                    8164.14.00 09/16  
07/20/2022                            09:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:49
02 Std. Gas	0.079	09:49
03 Room Air	RFI*	09:50
04 Room Air	0.000	09:50

\*Invalid Test  
Inhibited - RFI

Lot No = 02621080A1  
Cyl No = 35  
Exp Date = 03/05/2023  
County = 18                            Oper No. = 039947

 039947  
Operator Signature  
JONATHAN LAMPI

Remarks:

Form 106-I8000

Annual Inspection Install  
RFI Test