



ETHANOL GAS STANDARD CYLINDER REPORT

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM

SFN 59282 (08/2018)

Chemical Test Operator Name (Print) Dion Steinley		
Location Killdeer PD	Intoxilyzer® Serial Number 80-004938	
Gas Lot Number 34921080A1	Gas Cylinder Number 32	Gas Expiration Date 02/05/24

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
A. 0.080 AC
B. 0.080 AC
C. 0.080 AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature 	Date 2/24/2023
Reviewed By (Crime Laboratory Use Only) 	Date 13Mar2023


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004938
Location = KDPD 8164.14.00 09/16
02/24/2023 21:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:38
02 Std. Gas	0.080	21:39
03 Room Air	0.000	21:39
04 Std. Gas	0.080	21:39
05 Room Air	0.000	21:40
06 Std. Gas	0.080	21:40
07 Room Air	0.000	21:41

Lot No = 34921080A1
Cyl No = 32
Exp Date = 02/05/2024
County = 13 Oper No. = 120522

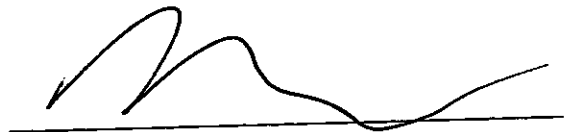

Operator Signature
DION STEINLEY

Remarks:

Form 106-I8000