



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number <u>80-006504</u>	Instrument Location <u>Wells Co. S.O.</u>
Reason for Install/Repair	
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): None 12 Apr 22
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date <u>02-Apr-22</u>
-------------------------------	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By <u>Janelle Putschner</u>	Certified Date <u>12 Apr 22</u>
---	------------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = WESO 8164.14.00 09/16
04/02/2022 09:37

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 26021080A1
Standard Cyl #? 30
Standard Expiration? 10/05/2023
Oper No? 131495

Flow Cal. Date: 08/20/2015
Slope 681
Intercept -673151

IR Calibration Date: 05/31/2017
 3um 9um

0th Coef(*100): -21488 -16160
1st Coef(*100): 265581 137324
2nd Coef(*100): 2507 1149
H2O adj(mg/l*10k): 519 348

***** Printer Test End *****

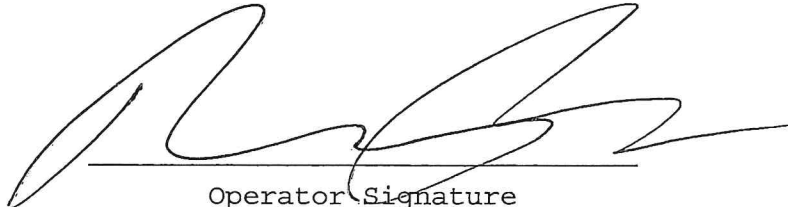

Operator Signature
MICHAEL BEAVER

Remarks:


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = WESO 8164.14.00 09/16
04/02/2022 10:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:14
02 Std. Gas	0.080	10:15
03 Room Air	0.000	10:15
04 Std. Gas	0.079	10:16
05 Room Air	0.000	10:16
06 Std. Gas	0.080	10:17
07 Room Air	0.000	10:17

Lot No = 26021080A1
Cyl No = 30
Exp Date = 10/05/2023
County = 52 Oper No. = 131495

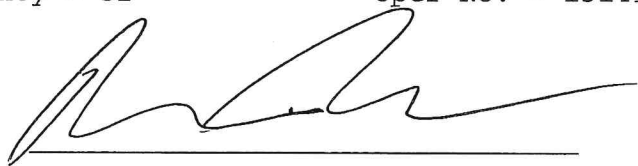

Operator Signature
MICHAEL BEAVER

Remarks:


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006504
Location = WESO 8164.14.00 09/16
04/02/2022 10:18

Test	AC	Time
01 Room Air	0.000	10:20
02 *Subject Test	RFI*	10:23
03 Room Air	0.000	10:23

*Invalid Test
Inhibited - RFI

Sub Name = TEST, TEST TEST
Sub DOB = 01/01/2000
Sub Sex = Male Weight = 150
Test = DUI Cit = 0000000
Dr. Lic. = ND/TEST0104940
Lot No = 26021080A1
Cyl No = 30
Expiration Date = 10/05/2023
County = 52 Oper No. = 131495

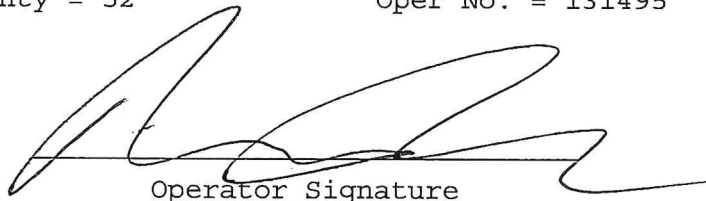

Operator Signature
MICHAEL BEAVER

Remarks: