



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
 SFN 59281 (06/2018)

Serial Number <b>80-006490</b>	Instrument Location <b>ASHL</b>
Reason for Install/Repair	
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): \_\_\_\_\_
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>Victor Fischer</i>	Date <b>3-13-2023</b>
---	-----------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By <i>Ann Muel</i>	Certified Date <b>16 Mar 23</b>
---------------------------------------	---------------------------------

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006490  
Location = ASHL                 8164.14.00 09/16  
03/13/2023                        16:53

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

Current Instrument Setup


Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?         1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            01923080A3  
Standard Cyl #?            62  
Standard Expiration?       02/05/2025  
Oper No?                    133262

Flow Cal. Date:            09/04/2020  
Slope                        649  
Intercept                   -598817

IR Calibration Date:        09/04/2020  
                                  3um                        9um

0th Coef(*100):	-25190	-16392
1st Coef(*100):	271645	136906
2nd Coef(*100):	2533	1222
H2O adj(mg/l*10k):	460	309

\*\*\*\*\* Printer Test End \*\*\*\*\*

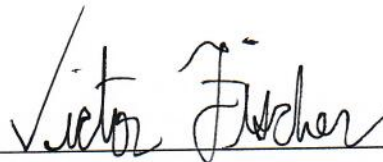

Operator Signature  
VICTOR FISCHER

Remarks:

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006490  
Location = ASHL                    8164.14.00 09/16  
03/13/2023                            17:14

Test	AC	Time
01 Room Air	0.000	17:16
02 *Subject Test	RFI*	17:16
03 Room Air	0.000	17:17

\*Invalid Test  
Inhibited - RFI

Sub Name = MMMM, MMMM MMMM  
Sub DOB = 01/01/1991  
Sub Sex = Female                    Weight = 200  
Test = DUI                            Cit = 000  
Dr. Lic. = ND/0000  
Lot No = 01923080A3  
Cyl No = 62  
Expiration Date = 02/05/2025  
County = 26                            Oper No. = 133262

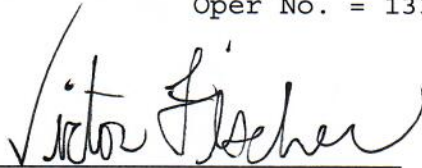

Operator Signature  
VICTOR FISCHER

Remarks:

Form 106-I8000