



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number 80-004199	Instrument Location Cass Jail - Machine #2
Reason for Install/Repair <input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) <u>Annual Inspection at Crime Laboratory</u>	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): None
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>Katherine M. Allen #3671</i>	Date 5-19-2023
--	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By <i>Aime Nahl</i>	Certified Date 22May2023
---	------------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = CASS 8164.14.00 09/16
05/19/2023 14:14

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

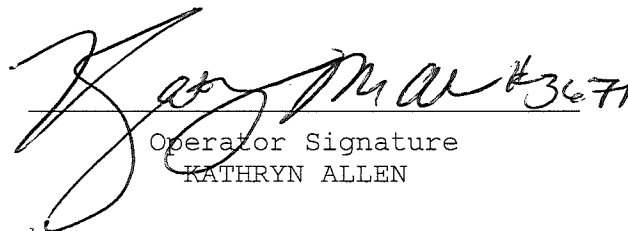
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 01923080A3
Standard Cyl #? 23
Standard Expiration? 02/05/2025
Oper No? 090801

Flow Cal. Date: 06/17/2019
Slope 593
Intercept -481610

IR Calibration Date: 06/17/2019
 3um 9um

0th Coef(*100): -17512 -19237
1st Coef(*100): 277207 136841
2nd Coef(*100): 1620 1027
H2O adj(mg/l*10k): 211 375

***** Printer Test End *****


Operator Signature
KATHRYN ALLEN

Remarks:

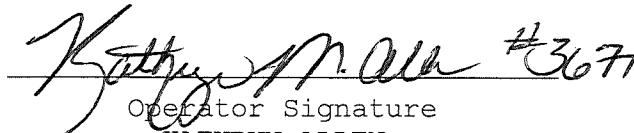
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = CASS 8164.14.00 09/16
05/19/2023 14:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:11
02 Std. Gas	0.082	14:11
03 Room Air	0.000	14:12
04 Std. Gas	0.080	14:12
05 Room Air	0.000	14:13
06 Std. Gas	0.082	14:13
07 Room Air	0.000	14:14

Lot No = 01923080A3
Cyl No = 23
Exp Date = 02/05/2025
County = 09 Oper No. = 090801

 #367
Operator Signature
KATHRYN ALLEN

Remarks:

Form 106-I8000

Instal New Machine
and gas canister


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = CASS 8164.14.00 09/16
05/19/2023 14:15

Test	AC	Time
01 Room Air	0.000	14:17
02 *Subject Test	RFI*	14:17
03 Room Air	RFI*	14:17

*Invalid Test
Inhibited - RFI

Sub Name = TEST, TEST NEW INSTAL NA
Sub DOB = 01/01/1900
Sub Sex = Female Weight = 145
Test = DUI Cit = NEW CAN INSTAL
Dr. Lic. = ND/NA
Lot No = 01923080A3
Cyl No = 23
Expiration Date = 02/05/2025
County = 09 Oper No. = 090801


Operator Signature
KATHRYN ALLEN

Remarks:

Form 106-I8000

*RFI Test for
New machine/Canister
Instal!*