



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

**INTOXILYZER® 8000 ANNUAL INSPECTION**

Intoxilyzer® 8000 Serial Number: 80-00 6499 Inspection Location: TOXL

**A. Pre-Inspection**

1. Items with Instrument:
  - Gas Cylinder  Yes or No (If Yes, Lot # 26021080A1 Cyl. # 10)
  - Keys  Yes or No
  - Power Cord  Yes or No
2.  Download Data
3.  Upload Operator File
4.  Current Location Code: JAME
5.  Battery Check
  - Was the external battery pack replaced? Yes or No
6.  O-Rings
  - Replaced Simulator O-Ring Yes or No
  - Replaced Breath Tube O-Ring Yes or No

**B. General Setup and Checks:**

1.  Diagnostics passed and instrument in "Ready" mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.  
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G).  
Display: 922 psi Regulator: 950 psi  
Display and Regulator ± 50 psi of each other Yes or No   
Gas tank tare necessary? Yes or No   
If Yes, display readings after tare (Level 3,M,C,G):  
Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

**C. Tests (Sign and attach test records):**

1.  Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - Low AC (Level 1,C)  
Known Value ≤ 0.03 AC: 0.020 AC  
Sim. Ser #: MP5318  
Lot #: 202201A  
Exp. Date: 11Jan24  
 Results ± 0.005 of known AC

Toxicology Unit - Breath Alcohol Section	Qualtrax ID: 11698 Revision: 1
Intoxilyzer 8000 Annual Inspection	Status: Published Published: 03/24/2023
UNCONTROLLED WHEN PRINTED	Page 1 of 2

2.  Configure simulator for the following test (Level 1,S).  
 Wet Calibration Check - High AC (Level 1,C)  
 Known Value  $\geq$  0.25 AC: 0.300 AC  
 Sim. Ser #: MP3067  
 Lot #: 202201F  
 Exp. Date: 18Jan24  
 Results  $\pm$  5% AC of known AC
3.  Configure dry gas standard for the remaining tests (Level 1,S).  
 Known Value : 0.080 AC  
 Gas Cylinder Lot #: 2602108041  
 Cylinder #: 3  
 Exp. Date: 10/5/23
4.  Interferent Check (Level 1,B)  
 Known Value: 0.10 AC + 0.05% Acetone  
 Sim. Ser #: DR7345  
 Lot #: ICS 7  
 Exp. Date: N/A  
 Display reads "Interferent Detect"
5.  RFI Check (CMS Mode)  
 Display reads "RFI Detect"
6.  Dry Calibration Check (Level 1,C)  
 Test 1 0.080    Test 4 0.080    Test 7 0.080  
 Test 2 0.079    Test 5 0.080    Test 8 0.080  
 Test 3 0.080    Test 6 0.080    Test 9 0.080  
 Average 0.079  
 Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: N/A

---



---

Instrument is acceptable to be used in the field. Yes or No  
 If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4.

[Signature]  
 Inspector Signature

07 June 2023  
 Date

Janelle Pertschiller  
 Reviewer

08 June 2023  
 Date

Toxicology Unit - Breath Alcohol Section	Qualtrax ID: 11698 Revision: 1
Intoxilyzer 8000 Annual Inspection	Status: Published Published: 03/24/2023
UNCONTROLLED WHEN PRINTED	Page 2 of 2

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006499  
Location = TOXL                    8164.14.00 09/16  
06/07/2023                            14:24

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup

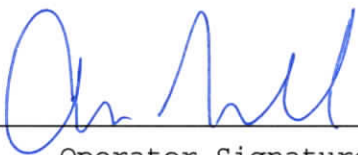
Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            26021080A1  
Standard Cyl #?            10  
Standard Expiration?       10/05/2023  
Oper No?                    133237

Flow Cal. Date:            08/18/2015  
Slope                        678  
Intercept                   -685002

IR Calibration Date:        08/18/2015  
                                  3um                            9um

-----  
0th Coef(\*100):            -22123                        -16014  
1st Coef(\*100):            264933                        138505  
2nd Coef(\*100):            3281                            1621  
H2O adj(mg/l\*10k):        704                            456

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks:    Print Test

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006499  
Location = TOXL      8164.14.00 09/16  
06/07/2023      14:29

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:30
02 Std. Sol.	0.020	14:31
03 Room Air	0.000	14:31
04 Std. Sol.	0.020	14:32
05 Room Air	0.000	14:32
06 Std. Sol.	0.020	14:33
07 Room Air	0.000	14:34

08 Sim Temp = 34.0°C

Simul Ser No = MP5318  
Std Sol No = 202201A  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: *LOW AC Check-0.020AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006499  
Location = TOXL      8164.14.00 09/16  
06/07/2023      14:40

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:41
02 Std. Sol.	0.299	14:42
03 Room Air	0.000	14:42
04 Std. Sol.	0.300	14:43
05 Room Air	0.000	14:44
06 Std. Sol.	0.299	14:45
07 Room Air	0.000	14:45

08 Sim Temp = 34.0°C

Simul Ser No = MP3067  
Std Sol No = 202201F  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: *High AC Check - 0.300Ac*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-006499  
Location = TOXL                              8164.14.00 09/16  
06/07/2023    14:46

Test	AC	Time
01 Room Air	0.000	14:47
02 *Subject Test	INT*	14:49
03 Room Air	0.000	14:50

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                                      Weight = NA  
Test = OTH                                      Cit = INTERFERENT CK  
Dr. Lic. = ND/TES989643  
Lot No = 26021080A1  
Cyl No = 3  
Expiration Date = 10/05/2023  
County = 08                                      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: *Interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

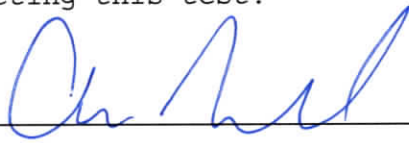
CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-006499  
Location = TOXL                      8164.14.00 09/16  
06/07/2023    14:50

Test	AC	Time
01 Diagnostic	OK	14:51
02 Room Air	0.000	14:51
03 *Subject Test	RFI*	14:52
04 Room Air	0.000	14:52

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                                      Weight = NA  
Test = OTH                                      Cit = RFI CHECK  
Dr. Lic. = ND/TES989643  
Lot No = 26021080A1  
Cyl No = 3  
Expiration Date = 10/05/2023  
County = 08                                      Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: *RFI check*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006499  
Location = TOXL      8164.14.00 09/16  
06/07/2023      14:52

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:53
02 Std. Gas	0.080	14:53
03 Room Air	0.000	14:54
04 Std. Gas	0.079	14:54
05 Room Air	0.000	14:55
06 Std. Gas	0.080	14:55
07 Room Air	0.000	14:56

Lot No = 26021080A1  
Cyl No = 3  
Exp Date = 10/05/2023  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000



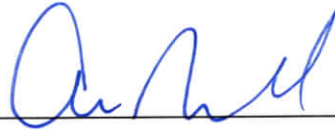
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006499  
Location = TOXL      8164.14.00 09/16  
06/07/2023      14:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:57
02 Std. Gas	0.080	14:57
03 Room Air	0.000	14:58
04 Std. Gas	0.080	14:58
05 Room Air	0.000	14:59
06 Std. Gas	0.080	14:59
07 Room Air	0.000	15:00

Lot No = 26021080A1  
Cyl No = 3  
Exp Date = 10/05/2023  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dry Cal check #4 to

Form 106-I8000

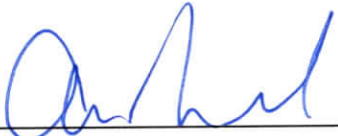
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006499  
Location = TOXL      8164.14.00 09/16  
06/07/2023      15:00

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:01
02 Std. Gas	0.080	15:01
03 Room Air	0.000	15:02
04 Std. Gas	0.080	15:02
05 Room Air	0.000	15:02
06 Std. Gas	0.080	15:03
07 Room Air	0.000	15:03

Lot No = 26021080A1  
Cyl No = 3  
Exp Date = 10/05/2023  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000