



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6671 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 34921080A1 Cyl. # 46)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: DEVL
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
 - Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
 - Display: 237 psi Regulator: 250 psi
 - Display and Regulator ± 50 psi of each other Yes or No
 - Gas tank tare necessary? Yes or No
 - If Yes, display readings after tare (Level 3,M,C,G):
 - Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
 - Wet Calibration Check - Low AC (Level 1,C)
 - Known Value ≤ 0.03 AC: 0.026 AC
 - Sim. Ser #: MP5318
 - Lot #: 202201A
 - Exp. Date: 1/Jan/24
 - Results ± 0.005 of known AC

| | |
|--|--|
| Toxicology Unit - Breath Alcohol Section | Qualtrax ID: 11698 Revision: 1 |
| Intoxilyzer 8000 Annual Inspection | Status: Published Published: 03/24/2023 |
| UNCONTROLLED WHEN PRINTED | Page 1 of 2 |

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.300 AC
 Sim. Ser #: MP3067
 Lot #: 202201F
 Exp. Date: 18Jan24
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 26021080 A1
 Cylinder #: 35
 Exp. Date: 10/5/23
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7345
 Lot #: ICS 7
 Exp. Date: N/A
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)
 Test 1 0.080 Test 4 0.080 Test 7 0.080
 Test 2 0.080 Test 5 0.081 Test 8 0.080
 Test 3 0.080 Test 6 0.080 Test 9 0.079
 Average 0.080
 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: Replaced Keyboard.

Instrument is acceptable to be used in the field. (Yes) or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4.

Ann Hill
 Inspector Signature

16 June 2023
 Date

Janelle Pertschauer
 Reviewer

19 June 2023
 Date

| | |
|--|--|
| Toxicology Unit - Breath Alcohol Section | Qualtrax ID: 11698 Revision: 1 |
| Intoxilyzer 8000 Annual Inspection | Status: Published Published: 03/24/2023 |
| UNCONTROLLED WHEN PRINTED | Page 2 of 2 |

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
06/16/2023 09:30

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34921080A1
Standard Cyl #? 46
Standard Expiration? 02/05/2024
Oper No? 133237

Flow Cal. Date: 08/22/2016
Slope 703
Intercept -691868

IR Calibration Date: 08/22/2016
 3um 9um

0th Coef(*100): -17135 -24345
1st Coef(*100): 254798 132856
2nd Coef(*100): 3386 1354
H2O adj(mg/l*10k): 610 539

***** Printer Test End *****

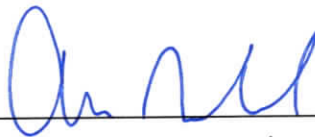

Operator Signature
ANNA NAREHOOD

Remarks: *Print Test*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
06/16/2023 09:45

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 09:46 |
| 02 Std. Sol. | 0.019 | 09:47 |
| 03 Room Air | 0.000 | 09:48 |
| 04 Std. Sol. | 0.019 | 09:48 |
| 05 Room Air | 0.000 | 09:49 |
| 06 Std. Sol. | 0.020 | 09:50 |
| 07 Room Air | 0.000 | 09:50 |

08 Sim Temp = 34.0°C

Simul Ser No = MP5318
Std Sol No = 202201A
County = 08 Oper No. = 133237

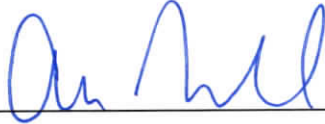

Operator Signature
ANNA NAREHOOD

Remarks: *LOW Ac Check - 0.020Ac*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
06/16/2023 09:51

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 09:52 |
| 02 Std. Sol. | 0.296 | 09:53 |
| 03 Room Air | 0.000 | 09:53 |
| 04 Std. Sol. | 0.296 | 09:54 |
| 05 Room Air | 0.000 | 09:54 |
| 06 Std. Sol. | 0.296 | 09:55 |
| 07 Room Air | 0.000 | 09:56 |


08 Sim Temp = 34.0°C

Simul Ser No = MP3067

Std Sol No = 202201F

County = 08

Oper No. = 133237

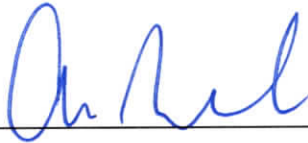

Operator Signature
ANNA NAREHOOD

Remarks:

High AC check - 0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
06/16/2023 09:59

| Test | AC | Time |
|------------------|-------|-------|
| 01 Room Air | 0.000 | 10:00 |
| 02 *Subject Test | INT* | 10:01 |
| 03 Room Air | 0.000 | 10:02 |

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 26021080A1
Cyl No = 35
Expiration Date = 10/05/2023
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Interferent Check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
06/16/2023 10:02

| Test | AC | Time |
|------------------|-------|-------|
| 01 Diagnostic | OK | 10:03 |
| 02 Room Air | 0.000 | 10:03 |
| 03 *Subject Test | RFI* | 10:04 |
| 04 Room Air | 0.000 | 10:04 |

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 26021080A1
Cyl No = 35
Expiration Date = 10/05/2023
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

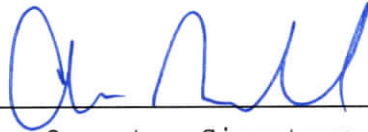

Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
06/16/2023 10:05

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 10:05 |
| 02 Std. Gas | 0.080 | 10:06 |
| 03 Room Air | 0.000 | 10:06 |
| 04 Std. Gas | 0.080 | 10:06 |
| 05 Room Air | 0.000 | 10:07 |
| 06 Std. Gas | 0.080 | 10:07 |
| 07 Room Air | 0.000 | 10:08 |

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry Cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
06/16/2023 10:09

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 10:09 |
| 02 Std. Gas | 0.080 | 10:10 |
| 03 Room Air | 0.000 | 10:10 |
| 04 Std. Gas | 0.081 | 10:10 |
| 05 Room Air | 0.000 | 10:11 |
| 06 Std. Gas | 0.080 | 10:11 |
| 07 Room Air | 0.000 | 10:12 |

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237

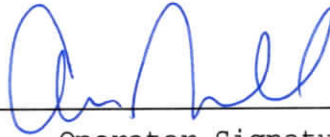

Operator Signature
ANNA NAREHOOD

Remarks: Dry Cal Check #4-6

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
06/16/2023 10:13

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 10:14 |
| 02 Std. Gas | 0.080 | 10:14 |
| 03 Room Air | 0.000 | 10:15 |
| 04 Std. Gas | 0.080 | 10:15 |
| 05 Room Air | 0.000 | 10:16 |
| 06 Std. Gas | 0.079 | 10:16 |
| 07 Room Air | 0.000 | 10:16 |

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000