



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4939 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # _____ Cyl. # _____)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: TOXL
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 553 psi Regulator: 550 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP5318
Lot #: 702201A
Exp. Date: 11/24/24
 Results ± 0.005 of known AC

Toxicology Unit - Breath Alcohol Section	Qualtrax ID: 11698 Revision: 1
Intoxilyzer 8000 Annual Inspection	Status: Published Published: 03/24/2023
UNCONTROLLED WHEN PRINTED	Page 1 of 2

- 2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.400 AC
 Sim. Ser #: MP3064
 Lot #: 202212C
 Exp. Date: 08Dec24
 Results \pm 5% AC of known AC
- 3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 26021080A1
 Cylinder #: 35
 Exp. Date: 10/5/23
- 4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7345
 Lot #: ICS7
 Exp. Date: NIA
 Display reads "Interferent Detect"
- 5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
- 6. Dry Calibration Check (Level 1,C)
 Test 1 0.079 Test 4 0.079 Test 7 0.080
 Test 2 0.079 Test 5 0.080 Test 8 0.079
 Test 3 0.080 Test 6 0.080 Test 9 0.079
 Average 0.079
 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No
 If No, state reason(s) why: _____

If Yes, change location code back to A.4.

[Signature]
 Inspector Signature

22 June 2023
 Date

[Signature]
 Reviewer

27 June 2023
 Date

Toxicology Unit - Breath Alcohol Section	Qualtrax ID: 11698 Revision: 1
Intoxilyzer 8000 Annual Inspection	Status: Published Published: 03/24/2023
UNCONTROLLED WHEN PRINTED	Page 2 of 2

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = WARD 8164.14.00 09/16
06/22/2023 12:19

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%\$^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%\$^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 34418080A2
Standard Cyl #? 52
Standard Expiration? 02/05/2021
Oper No? 133237

Flow Cal. Date: 01/18/2010
Slope 724
Intercept -779308

IR Calibration Date: 06/22/2023
 3um 9um

0th Coef(*100): -19230 -17600
1st Coef(*100): 257947 133671
2nd Coef(*100): 3268 1535
H2O adj(mg/l*10k): 529 419

***** Printer Test End *****

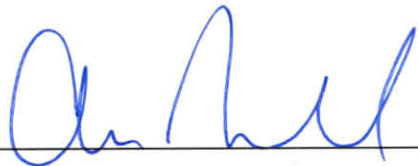

Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = WARD 8164.14.00 09/16
06/22/2023 12:22

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:22
02 Std. Sol.	0.020	12:25
03 Room Air	0.000	12:26
04 Std. Sol.	0.020	12:27
05 Room Air	0.000	12:27
06 Std. Sol.	0.020	12:28
07 Room Air	0.000	12:28

08 Sim Temp = 34.0°C

Simul Ser No = MP5318

Std Sol No = 202201A

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *LOW AC Check - 0.020AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = WARD 8164.14.00 09/16
06/22/2023 12:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:35
02 Std. Sol.	0.411	12:36
03 Room Air	0.000	12:37
04 Std. Sol.	0.411	12:37
05 Room Air	0.000	12:38
06 Std. Sol.	0.411	12:39
07 Room Air	0.000	12:39

08 Sim Temp = 34.0°C

Simul Ser No = MP3069

Std Sol No = 202212C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC Check - 0.400Ac

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = WARD 8164.14.00 09/16
06/22/2023 12:44

Test	AC	Time
01 Diagnostic	OK	12:45
02 Room Air	0.000	12:46
03 *Subject Test	RFI*	12:46
04 Room Air	0.000	12:46

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 26021080A1
Cyl No = 35
Expiration Date = 10/05/2023
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

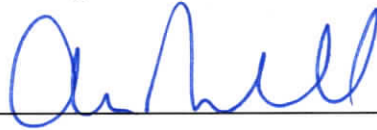

Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = WARD 8164.14.00 09/16
06/22/2023 12:47

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:47
02 Std. Gas	0.079	12:48
03 Room Air	0.000	12:48
04 Std. Gas	0.079	12:48
05 Room Air	0.000	12:49
06 Std. Gas	0.080	12:49
07 Room Air	0.000	12:50

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = WARD 8164.14.00 09/16
06/22/2023 12:50

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:51
02 Std. Gas	0.079	12:51
03 Room Air	0.000	12:52
04 Std. Gas	0.080	12:52
05 Room Air	0.000	12:53
06 Std. Gas	0.080	12:53
07 Room Air	0.000	12:53

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237

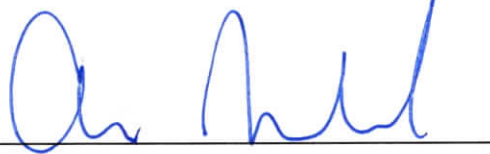

Operator Signature
ANNA NAREHOOD

Remarks: Dry Cal Check #4-c

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = WARD 8164.14.00 09/16
06/22/2023 12:54

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:54
02 Std. Gas	0.080	12:54
03 Room Air	0.000	12:55
04 Std. Gas	0.079	12:55
05 Room Air	0.000	12:56
06 Std. Gas	0.079	12:56
07 Room Air	0.000	12:57

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237

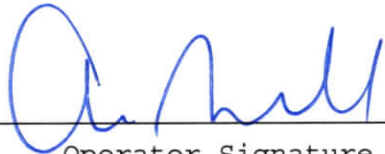

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000