



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
 SFN 59281 (06/2018)

Serial Number <b>80-006500</b>	Instrument Location <b>Harvey Police Department</b>
Reason for Install/Repair	
<input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) <b>Annual Inspection at Crime Laboratory</b>	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): **N/A**
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

*All forms sent in. AEW*

Field Inspector Signature 	Date <b>6/23/2023</b>
-------------------------------	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By 	Certified Date <b>27 June 2023</b>
---------------------------	---------------------------------------

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006500  
Location = HARV                 8164.14.00 09/16  
06/23/2023                        16:38

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-==|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-==|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

Current Instrument Setup


Data Entry Mode:                Enabled  
Start Test Sequence:            DABACABA  
Display Prelim Rslt?            Yes  
Display Third Digit?            Yes  
Inhib Printer(Y/N)?            No  
Display Volume?                No  
Disable On Memfull?            Yes  
# of Print Copies?              1  
Select Std (D/W/I)?            Dry  
Standard Value?                0.080  
Standard Lot #?                 01923080A3  
Standard Cyl #?                 59  
Standard Expiration?            02/05/2025  
Oper No?                        133314

Flow Cal. Date:                 08/18/2015  
Slope                            681  
Intercept                        -680985

IR Calibration Date:            08/18/2015  
                                    3um                            9um

-----  
0th Coef(\*100):                -3148                        -17259  
1st Coef(\*100):                254475                      138520  
2nd Coef(\*100):                1954                         1329  
H2O adj(mg/l\*10k):            193                          414

\*\*\*\*\* Printer Test End \*\*\*\*\*

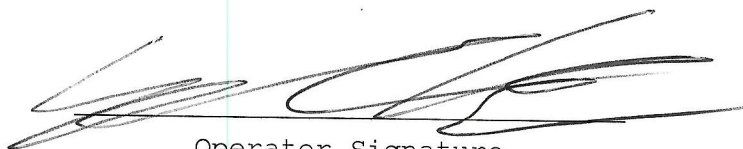

Operator Signature  
SPENCER VOLK

Remarks:

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006500  
Location = HARV                    8164.14.00 09/16  
06/23/2023                            16:39

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:40
02 Std. Gas	0.080	16:40
03 Room Air	0.000	16:41
04 Std. Gas	0.080	16:41
05 Room Air	0.000	16:42
06 Std. Gas	0.080	16:42
07 Room Air	0.000	16:43

Lot No = 01923080A3  
Cyl No = 59  
Exp Date = 02/05/2025  
County = 52                            Oper No. = 133314

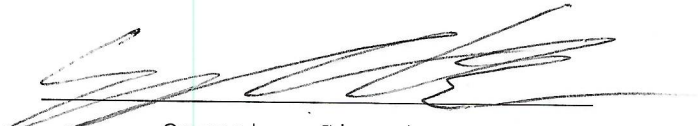  
Operator Signature  
SPENCER VOLK

Remarks:


Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006500  
Location = HARV                 8164.14.00 09/16  
06/23/2023                        16:44

Test	AC	Time
01 Room Air	0.000	16:47
02 *Subject Test	RFI*	16:48
03 Room Air	0.000	16:48

\*Invalid Test  
Inhibited - RFI

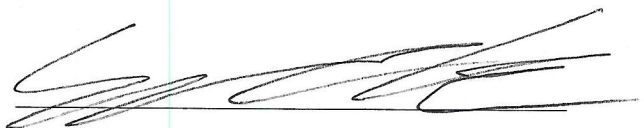

Operator Signature  
SPENCER VOLK

Remarks: RFI Test

Form 106-I8000