



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6687 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 34921080A1 Cyl. # 34)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: PLPD
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 976 psi Regulator: 1060 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP5318
Lot #: 202201A
Exp. Date: 11/24/24
 Results ± 0.005 of known AC

Toxicology Unit - Breath Alcohol Section	Qualtrax ID: 11698 Revision: 1
Intoxilyzer 8000 Annual Inspection	Status: Published Published: 03/24/2023
UNCONTROLLED WHEN PRINTED	Page 1 of 2

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.300 AC
 Sim. Ser #: 202201F MP3067
 Lot #: ~~18Jan21~~ 202201F 30June23
 Exp. Date: 18Jan24
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 26021080A1
 Cylinder #: 35
 Exp. Date: 10/5/23
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7345
 Lot #: ICS 7
 Exp. Date: NIA
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)

Test 1 <u>0.080</u>	Test 4 <u>0.080</u>	Test 7 <u>0.080</u>
Test 2 <u>0.080</u>	Test 5 <u>0.080</u>	Test 8 <u>0.080</u>
Test 3 <u>0.080</u>	Test 6 <u>0.080</u>	Test 9 <u>0.080</u>
Average <u>0.080</u>		

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4.

[Signature]
 Inspector Signature

28 June 2023
 Date

[Signature]
 Reviewer

30 June 2023
 Date

Toxicology Unit - Breath Alcohol Section	Qualtrax ID: 11698 Revision: 1
Intoxilyzer 8000 Annual Inspection	Status: Published Published: 03/24/2023
UNCONTROLLED WHEN PRINTED	Page 2 of 2

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
06/28/2023 13:50

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Wet
Standard Value? 0.020
Standard Solution #? 202201A
Sim Serial #? MP5318
Oper No? 133237

Flow Cal. Date: 10/05/2018
Slope 696
Intercept -609977

IR Calibration Date: 10/05/2018
 3um 9um

0th Coef(*100):	-11478	-18771
1st Coef(*100):	255256	132135
2nd Coef(*100):	4432	1676
H2O adj(mg/l*10k):	604	575

***** Printer Test End *****



Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
06/28/2023 13:51


WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:51
02 Std. Sol.	0.020	13:52
03 Room Air	0.000	13:53
04 Std. Sol.	0.020	13:53
05 Room Air	0.000	13:54
06 Std. Sol.	0.020	13:55
07 Room Air	0.000	13:55

08 Sim Temp = 34.0°C

Simul Ser No = MP5318
Std Sol No = 202201A
County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Low Ac Check -0.020Ac

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
06/28/2023 13:56

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:57
02 Std. Sol.	0.299	13:58
03 Room Air	0.000	13:58
04 Std. Sol.	0.300	13:59
05 Room Air	0.000	14:00
06 Std. Sol.	0.300	14:00
07 Room Air	0.000	14:01

08 Sim Temp = 34.0°C

Simul Ser No = MP3067
Std Sol No = 202201F
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High Ac Check-0.300Ac

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
06/28/2023 14:03

Test	AC	Time
01 Room Air	0.000	14:04
02 *Subject Test	INT*	14:04
03 Room Air	0.000	14:05

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 26021080A1
Cyl No = 35
Expiration Date = 10/05/2023
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Interferent Check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
06/28/2023 14:05

Test	AC	Time
01 Diagnostic	OK	14:06
02 Room Air	0.000	14:06
03 *Subject Test	RFI*	14:07
04 Room Air	0.000	14:07

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 26021080A1
Cyl No = 35
Expiration Date = 10/05/2023
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

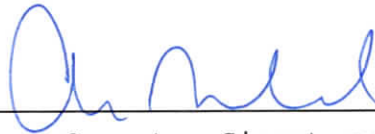

Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
06/28/2023 14:08

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:08
02 Std. Gas	0.080	14:09
03 Room Air	0.000	14:09
04 Std. Gas	0.080	14:10
05 Room Air	0.000	14:10
06 Std. Gas	0.080	14:11
07 Room Air	0.000	14:11

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
06/28/2023 14:12

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:12
02 Std. Gas	0.080	14:13
03 Room Air	0.000	14:13
04 Std. Gas	0.080	14:13
05 Room Air	0.000	14:14
06 Std. Gas	0.080	14:14
07 Room Air	0.000	14:15

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
06/28/2023 14:15

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:16
02 Std. Gas	0.080	14:16
03 Room Air	0.000	14:16
04 Std. Gas	0.080	14:17
05 Room Air	0.000	14:17
06 Std. Gas	0.080	14:18
07 Room Air	0.000	14:18

Lot No = 26021080A1
Cyl No = 35
Exp Date = 10/05/2023
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry Cal check #7-9

Form 106-I8000