




INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number 80-006508	Instrument Location RICHLAND COUNTY JAIL
Reason for Install/Repair <input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) INSTALL DUE TO NON-DETECTION OF EXTERNAL PRINTER	


Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): _____
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date 07/05/2023
------------------------------------------------------------------------------------------------------------------	---------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By 	Certified Date 10/10/23
--------------------------------------------------------------------------------------------------------------	-----------------------------------

*emailed
 *called Chris Hurd on 10/12 to inform
 him that a reinstall is not
 necessary to reconnect the external
 printer. aew*

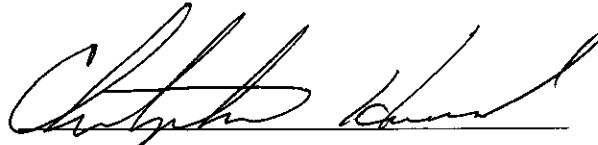
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006508
Location = WAHP 8164.14.00 09/16
07/05/2023 11:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:56
02 Std. Gas	0.080	11:57
03 Room Air	0.000	11:57
04 Std. Gas	0.080	11:58
05 Room Air	0.000	11:58
06 Std. Gas	0.079	11:59
07 Room Air	0.000	11:59

Lot No = 34921080A1
Cyl No = 35
Exp Date = 02/05/2024
County = 39 Oper No. = 132570



Operator Signature
CHRISTOPHER HUARD

Remarks: *ALA; GOOD*

Form 106-I8000

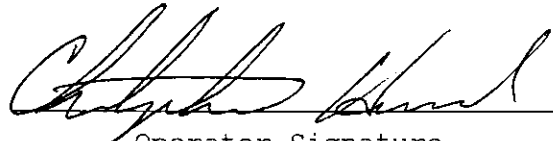
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006508
Location = WAHP 8164.14.00 09/16
07/05/2023 12:00

Test	AC	Time
01 Room Air	RFI*	12:01
02 Room Air	0.000	12:02

*Invalid Test
Inhibited - RFI

Sub Name = DOE, JOHN NA
Sub DOB = 01/01/1980
Sub Sex = Male Weight = 215
Test = DUI Cit = 123456789
Dr. Lic. = ND/DOE803432
Lot No = 34921080A1
Cyl No = 35
Expiration Date = 02/05/2024
County = 39 Oper No. = 132570


Operator Signature
CHRISTOPHER HUARD

Remarks: RFI ; (GOOD)

Form 106-I8000