



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6691 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
  - Gas Cylinder  Yes or No (If Yes, Lot # 01923080A3 Cyl. # 61)
  - Keys  Yes or No
  - Power Cord  Yes or No
2.  Download Data
3.  Upload Operator File
4.  Current Location Code: KMPD
5.  Battery Check
  - Was the external battery pack replaced?  Yes or No
6.  O-Rings
  - Replaced Simulator O-Ring  Yes or No
  - Replaced Breath Tube O-Ring  Yes or No

B. General Setup and Checks:

1.  Diagnostics passed and instrument in "Ready" mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.  
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G).  
Display: 928 psi Regulator: 975 psi  
Display and Regulator ± 50 psi of each other  Yes or No  
Gas tank tare necessary?  Yes or No  
If Yes, display readings after tare (Level 3,M,C,G):  
Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

C. Tests (Sign and attach test records):

1.  Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - Low AC (Level 1,C)  
Known Value ≤ 0.03 AC: 0.020 AC  
Sim. Ser #: MP3002  
Lot #: 202301E  
Exp. Date: 17 Jan 25  
 Results ± 0.005 of known AC

2.  Configure simulator for the following test (Level 1,S).  
 Wet Calibration Check - High AC (Level 1,C)  
 Known Value  $\geq$  0.25 AC: 0.400 AC  
 Sim. Ser #: MP6036  
 Lot #: 202212C  
 Exp. Date: 08 Dec 24  
 Results  $\pm$  5% AC of known AC
3.  Configure dry gas standard for the remaining tests (Level 1,S).  
 Known Value : 0.080 AC  
 Gas Cylinder Lot #: 14323080A4  
 Cylinder #: 13  
 Exp. Date: 6/5/25
4.  Interferent Check (Level 1,B)  
 Known Value: 0.10 AC + 0.05% Acetone  
 Sim. Ser #: DR7344  
 Lot #: ICS 8  
 Exp. Date: NIA  
 Display reads "Interferent Detect"
5.  RFI Check (CMS Mode)  
 Display reads "RFI Detect"
6.  Dry Calibration Check (Level 1,C)
 

Test 1	<u>0.079</u>	Test 4	<u>0.080</u>	Test 7	<u>0.079</u>
Test 2	<u>0.080</u>	Test 5	<u>0.079</u>	Test 8	<u>0.079</u>
Test 3	<u>0.080</u>	Test 6	<u>0.079</u>	Test 9	<u>0.079</u>
Average <u>0.079</u>					

 Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: Ran 6 dry cal checks, values were running high so a calibration adjustment was performed. Low AC, high AC and all dry calibration checks were reran.

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4.  NIA instrument swapped.

[Signature]  
 Inspector Signature

03 Apr 2024  
 Date

[Signature]  
 Reviewer

04 Apr 2024  
 Date



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/02/2024      14:04

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:05
02 Std. Sol.	0.020	14:06
03 Room Air	0.000	14:07
04 Std. Sol.	0.020	14:08
05 Room Air	0.000	14:08
06 Std. Sol.	0.020	14:09
07 Room Air	0.000	14:09

08 Sim Temp = 34.0°C

Simul Ser No = MP3002  
Std Sol No = 202301E  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: LOW AC check - 0.020AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/02/2024      14:15

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:16
02 Std. Sol.	0.404	14:17
03 Room Air	0.000	14:17
04 Std. Sol.	0.405	14:18
05 Room Air	0.000	14:18
06 Std. Sol.	0.405	14:19
07 Room Air	0.000	14:20

08 Sim Temp = 34.0°C

Simul Ser No = MP6036  
Std Sol No = 202212C  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: High cal check - 0.400AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006691  
Location = TOXL                    8164.14.00 09/16  
04/02/2024                            14:21

Test	AC	Time
01 Room Air	0.000	14:22
02 *Subject Test	INT*	14:22
03 Room Air	0.000	14:23

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                      Weight = NA  
Test = OTH                          Cit = INTERFERENT CK  
Dr. Lic. = ND/TES989643  
Lot No = 14323080A4  
Cyl No = 13  
Expiration Date = 06/05/2025  
County = 08                          Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: *interferent check*

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/02/2024      14:26

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:26
02 Std. Gas	0.083	14:27
03 Room Air	0.000	14:27
04 Std. Gas	0.082	14:27
05 Room Air	0.000	14:28
06 Std. Gas	0.083	14:28
07 Room Air	0.000	14:29

Lot No = 14323080A4  
Cyl No = 13  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #1-3  
cal adj needed

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/02/2024      14:29

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:30
02 Std. Gas	0.083	14:30
03 Room Air	0.000	14:31
04 Std. Gas	0.083	14:31
05 Room Air	0.000	14:32
06 Std. Gas	0.083	14:32
07 Room Air	0.000	14:32

Lot No = 14323080A4  
Cyl No = 13  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dry Cal check #4-6  
pre cal adj.

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/03/2024      09:12

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:12
02 Std. Sol.	0.019	09:13
03 Room Air	0.000	09:14
04 Std. Sol.	0.019	09:14
05 Room Air	0.000	09:15
06 Std. Sol.	0.020	09:15
07 Room Air	0.000	09:16


08 Sim Temp = 34.0°C

Simul Ser No = MP3002

Std Sol No = 202301E

County = 08

Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: *Low Ac Check - 0.020AC  
Post calibration adjustment.*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/03/2024      09:29

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:29
02 Std. Sol.	0.397	09:30
03 Room Air	0.000	09:30
04 Std. Sol.	0.399	09:31
05 Room Air	0.000	09:32
06 Std. Sol.	0.399	09:32
07 Room Air	0.000	09:33

08 Sim Temp = 34.0°C

Simul Ser No = MP6036

Std Sol No = 202212C

County = 08

Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks:

High Ae Check - 0.400Ac  
Post calibration adjustment

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/03/2024      09:35

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:35
02 Std. Gas	0.079	09:35
03 Room Air	0.000	09:36
04 Std. Gas	0.080	09:36
05 Room Air	0.000	09:37
06 Std. Gas	0.080	09:37
07 Room Air	0.000	09:38

Lot No = 14323080A4  
Cyl No = 13  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dny Cal check #1-3  
Post cal adj.

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/03/2024      09:38

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:39
02 Std. Gas	0.080	09:39
03 Room Air	0.000	09:39
04 Std. Gas	0.079	09:40
05 Room Air	0.000	09:40
06 Std. Gas	0.079	09:41
07 Room Air	0.000	09:41

Lot No = 14323080A4  
Cyl No = 13  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #4-6  
post cal adj.

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006691  
Location = TOXL      8164.14.00 09/16  
04/03/2024      09:41

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:42
02 Std. Gas	0.079	09:42
03 Room Air	0.000	09:43
04 Std. Gas	0.079	09:43
05 Room Air	0.000	09:44
06 Std. Gas	0.079	09:44
07 Room Air	0.000	09:45

Lot No = 14323080A4  
Cyl No = 13  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237

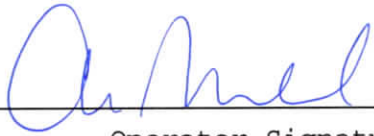  
Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #7-9  
post cal adj.

Form 106-I8000