




INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number 80-004956	Instrument Location CCSO
Reason for Install/Repair	
<input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) Annual Inspection at Crime Laboratory	


Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): _____
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date 13-Apr-24
--	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By 	Certified Date 16April2024
--	--------------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = COOP 8164.14.00 09/16
04/09/2024 10:10

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 14323080A1
Standard Cyl #? 70
Standard Expiration? 06/05/2025
Oper No? 131495

Flow Cal. Date: 06/13/2019
Slope 606
Intercept -586035

IR Calibration Date: 06/13/2019
 3um 9um

	3um	9um
0th Coef(*100):	-19986	-21891
1st Coef(*100):	263289	136002
2nd Coef(*100):	2309	1332
H2O adj(mg/l*10k):	544	502

***** Printer Test End *****

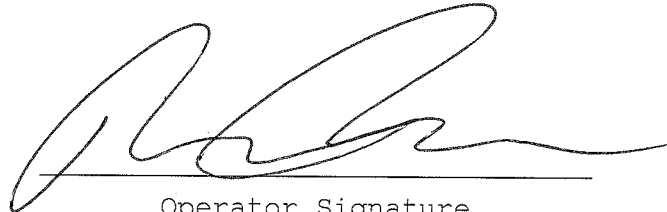

Operator Signature
MICHAEL BEAVER

Remarks: Good

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = COOP 8164.14.00 09/16
04/09/2024 10:19

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:20
02 Std. Gas	0.081	10:20
03 Room Air	0.000	10:21
04 Std. Gas	0.082	10:21
05 Room Air	0.000	10:22
06 Std. Gas	0.082	10:22
07 Room Air	0.000	10:22

Lot No = 14323080A1
Cyl No = 70
Exp Date = 06/05/2025
County = 20 Oper No. = 131495

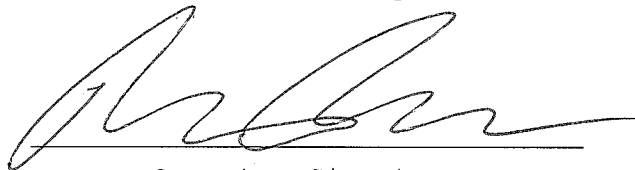

Operator Signature
MICHAEL BEAVER

Remarks: *Good*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = COOP 8164.14.00 09/16
04/09/2024 10:26

Test	AC	Time
01 Room Air	RFI*	10:27
02 Room Air	0.000	10:27

*Invalid Test
Inhibited - RFI

Sub Name = TEST, TEST TEST
Sub DOB = 01/01/1990
Sub Sex = Male Weight = 100
Test = OTH Cit = 00
Dr. Lic. = ND/TEST
Lot No = 14323080A1
Cyl No = 70
Expiration Date = 06/05/2025
County = 20 Oper No. = 131495



Operator Signature
MICHAEL BEAVER

Remarks: *Good RFI*

Form 106-I8000